

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

**Calibration of tuneable laser sources**

**Étalonnage des sources laser accordables**

IECNORM.COM : Click to view the full PDF of IEC 62522:2024



## THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2024 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'IEC ou du Comité national de l'IEC du pays du demandeur. Si vous avez des questions sur le copyright de l'IEC ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de l'IEC de votre pays de résidence.

IEC Secretariat  
3, rue de Varembe  
CH-1211 Geneva 20  
Switzerland

Tel.: +41 22 919 02 11  
[info@iec.ch](mailto:info@iec.ch)  
[www.iec.ch](http://www.iec.ch)

### About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

### About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

#### IEC publications search - [webstore.iec.ch/advsearchform](http://webstore.iec.ch/advsearchform)

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee, ...). It also gives information on projects, replaced and withdrawn publications.

#### IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

#### IEC Customer Service Centre - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: [sales@iec.ch](mailto:sales@iec.ch).

#### IEC Products & Services Portal - [products.iec.ch](http://products.iec.ch)

Discover our powerful search engine and read freely all the publications previews, graphical symbols and the glossary. With a subscription you will always have access to up to date content tailored to your needs.

#### Electropedia - [www.electropedia.org](http://www.electropedia.org)

The world's leading online dictionary on electrotechnology, containing more than 22 500 terminological entries in English and French, with equivalent terms in 25 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

### A propos de l'IEC

La Commission Electrotechnique Internationale (IEC) est la première organisation mondiale qui élabore et publie des Normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

### A propos des publications IEC

Le contenu technique des publications IEC est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

#### Recherche de publications IEC -

[webstore.iec.ch/advsearchform](http://webstore.iec.ch/advsearchform)

La recherche avancée permet de trouver des publications IEC en utilisant différents critères (numéro de référence, texte, comité d'études, ...). Elle donne aussi des informations sur les projets et les publications remplacées ou retirées.

#### IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)

Restez informé sur les nouvelles publications IEC. Just Published détaille les nouvelles publications parues. Disponible en ligne et une fois par mois par email.

#### Service Clients - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions contactez-nous: [sales@iec.ch](mailto:sales@iec.ch).

#### IEC Products & Services Portal - [products.iec.ch](http://products.iec.ch)

Découvrez notre puissant moteur de recherche et consultez gratuitement tous les aperçus des publications, symboles graphiques et le glossaire. Avec un abonnement, vous aurez toujours accès à un contenu à jour adapté à vos besoins.

#### Electropedia - [www.electropedia.org](http://www.electropedia.org)

Le premier dictionnaire d'électrotechnologie en ligne au monde, avec plus de 22 500 articles terminologiques en anglais et en français, ainsi que les termes équivalents dans 25 langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International (IEV) en ligne.

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

Calibration of tuneable laser sources

Étalonnage des sources laser accordables

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

COMMISSION  
ELECTROTECHNIQUE  
INTERNATIONALE

ICS 31.260, 33.180.01

ISBN 978-2-8322-9034-7

**Warning! Make sure that you obtained this publication from an authorized distributor.**  
**Attention! Veuillez vous assurer que vous avez obtenu cette publication via un distributeur agréé.**

## CONTENTS

|                                                                                      |    |
|--------------------------------------------------------------------------------------|----|
| FOREWORD.....                                                                        | 4  |
| INTRODUCTION.....                                                                    | 6  |
| 1 Scope.....                                                                         | 7  |
| 2 Normative references .....                                                         | 7  |
| 3 Terms, definitions, and abbreviated terms .....                                    | 7  |
| 3.1 Terms and definitions.....                                                       | 7  |
| 3.2 Abbreviated terms.....                                                           | 10 |
| 4 Preparation for calibration .....                                                  | 10 |
| 4.1 Organization .....                                                               | 10 |
| 4.2 Traceability .....                                                               | 10 |
| 4.3 Preparation .....                                                                | 10 |
| 4.4 Reference calibration conditions .....                                           | 11 |
| 5 Wavelength calibration .....                                                       | 11 |
| 5.1 Overview.....                                                                    | 11 |
| 5.2 Wavelength calibration at reference conditions .....                             | 12 |
| 5.2.1 Set-up .....                                                                   | 12 |
| 5.2.2 Calibration equipment.....                                                     | 12 |
| 5.2.3 Procedure for wavelength calibration .....                                     | 12 |
| 5.2.4 Dependence on conditions.....                                                  | 13 |
| 5.2.5 Uncertainty at reference conditions.....                                       | 15 |
| 5.3 Wavelength calibration at operating conditions .....                             | 16 |
| 5.3.1 General .....                                                                  | 16 |
| 5.3.2 Optical power dependence .....                                                 | 16 |
| 5.3.3 Uncertainty at operating conditions .....                                      | 17 |
| 6 Optical power calibration .....                                                    | 18 |
| 6.1 Overview.....                                                                    | 18 |
| 6.2 Optical power calibration at reference conditions .....                          | 18 |
| 6.2.1 Set-up .....                                                                   | 18 |
| 6.2.2 Calibration equipment.....                                                     | 19 |
| 6.2.3 Procedure for power calibration at reference conditions.....                   | 19 |
| 6.2.4 Dependence on conditions.....                                                  | 20 |
| 6.2.5 Uncertainty at reference conditions.....                                       | 23 |
| 6.3 Optical power calibration at operating conditions .....                          | 23 |
| 6.3.1 General .....                                                                  | 23 |
| 6.3.2 Wavelength dependence .....                                                    | 24 |
| 6.3.3 Uncertainty at operating conditions .....                                      | 25 |
| 7 Documentation .....                                                                | 25 |
| 7.1 Calibration data and uncertainty.....                                            | 25 |
| 7.2 Calibration conditions .....                                                     | 26 |
| Annex A (normative) Mathematical basis for measurement uncertainty calculations..... | 27 |
| A.1 General.....                                                                     | 27 |
| A.2 Type A evaluation of uncertainty .....                                           | 27 |
| A.3 Type B evaluation of uncertainty .....                                           | 28 |
| A.4 Determining the combined standard uncertainty.....                               | 29 |
| A.5 Reporting.....                                                                   | 29 |
| Annex B (informative) Other testing .....                                            | 30 |

|                       |                                                                                     |    |
|-----------------------|-------------------------------------------------------------------------------------|----|
| B.1                   | General.....                                                                        | 30 |
| B.2                   | Wavelength tuning resolution .....                                                  | 30 |
| B.2.1                 | Set-up .....                                                                        | 30 |
| B.2.2                 | Testing equipment .....                                                             | 30 |
| B.2.3                 | Testing procedure for determining wavelength resolution.....                        | 30 |
| B.3                   | Optical power tuning resolution .....                                               | 31 |
| B.3.1                 | Set-up .....                                                                        | 31 |
| B.3.2                 | Testing equipment .....                                                             | 31 |
| B.3.3                 | Testing procedure for optical power resolution .....                                | 31 |
| B.4                   | Signal-to-source spontaneous emission ratio .....                                   | 32 |
| B.4.1                 | General .....                                                                       | 32 |
| B.4.2                 | Set-up .....                                                                        | 32 |
| B.4.3                 | Testing equipment .....                                                             | 32 |
| B.4.4                 | Testing procedure for determining signal-to-source spontaneous emission ratio ..... | 32 |
| B.5                   | Side-mode suppression ratio.....                                                    | 33 |
| B.5.1                 | General .....                                                                       | 33 |
| B.5.2                 | Set-up .....                                                                        | 33 |
| B.5.3                 | Testing equipment .....                                                             | 34 |
| B.5.4                 | Testing procedure for determining the side-mode suppression ratio.....              | 34 |
| Annex C (informative) | Linear to dB scale conversion of uncertainties.....                                 | 37 |
| C.1                   | Definition of decibel .....                                                         | 37 |
| C.2                   | Conversion of relative uncertainties .....                                          | 37 |
| Bibliography          | .....                                                                               | 39 |
| Figure 1              | – Measurement set-up for wavelength calibration.....                                | 12 |
| Figure 2              | – Measurement set-up for temperature dependence.....                                | 13 |
| Figure 3              | – Measurement set-up for wavelength stability .....                                 | 14 |
| Figure 4              | – Measurement set-up for optical power dependence.....                              | 16 |
| Figure 5              | – Measurement set-up for intrinsic optical power calibration.....                   | 18 |
| Figure 6              | – Measurement set-up for temperature dependence.....                                | 20 |
| Figure 7              | – Measurement set-up for optical power stability.....                               | 21 |
| Figure 8              | – Measurement set-up for connection repeatability/reproducibility .....             | 22 |
| Figure 9              | – Measurement set-up for wavelength dependence .....                                | 24 |
| Figure B.1            | – Measurement set-up for wavelength resolution .....                                | 30 |
| Figure B.2            | – Measurement set-up for optical power resolution setting test .....                | 31 |
| Figure B.3            | – Measurement set-up for signal to total source spontaneous emission ratio .....    | 32 |
| Figure B.4            | – Measurement of the signal to spontaneous emission ratio.....                      | 33 |
| Figure B.5            | – Measurement set-up for the side-mode suppression ratio test.....                  | 33 |
| Figure B.6            | – Optical spectrum of tuneable laser source .....                                   | 35 |
| Figure B.7            | – Measurement set-up for SMSR .....                                                 | 35 |
| Table 1               | – Source of uncertainty for wavelength calibration.....                             | 11 |
| Table 2               | – Source of uncertainty for optical power calibration.....                          | 18 |

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

## CALIBRATION OF TUNEABLE LASER SOURCES

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) IEC draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). IEC takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, IEC had not received notice of (a) patent(s), which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at <https://patents.iec.ch>. IEC shall not be held responsible for identifying any or all such patent rights.

IEC 62522 has been prepared by IEC technical committee 86: Fibre optics. It is an International Standard.

This second edition cancels and replaces the first edition published in 2014. This edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- a) addition of references to IEC 61315;
- b) addition of Table 1 and Table 2 on uncertainties;
- c) clarification of the reference power meter settings in 6.2.3 and 6.3.2.3.

The text of this International Standard is based on the following documents:

| Draft       | Report on voting |
|-------------|------------------|
| 86/639/FDIS | 86/643/RVD       |

Full information on the voting for its approval can be found in the report on voting indicated in the above table.

The language used for the development of this International Standard is English.

This document was drafted in accordance with ISO/IEC Directives, Part 2, and developed in accordance with ISO/IEC Directives, Part 1 and ISO/IEC Directives, IEC Supplement, available at [www.iec.ch/members\\_experts/refdocs](http://www.iec.ch/members_experts/refdocs). The main document types developed by IEC are described in greater detail at [www.iec.ch/publications](http://www.iec.ch/publications).

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under [webstore.iec.ch](http://webstore.iec.ch) in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn, or
- revised.

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## INTRODUCTION

Wavelength-division multiplexing (WDM) transmission systems have been deployed in optical trunk lines. ITU-T Recommendations in the G.694 series describe the frequency and wavelength grids for WDM applications. For example, the frequency grid of ITU-T Recommendation G.694.1 supports a variety of channel spacing ranging from 12,5 GHz to 100 GHz and wider. WDM devices, such as arrayed waveguide grating (AWG), thin film filter or grating based multiplexers (MUX), and demultiplexers (DMUX) with narrow channel spacing are incorporated in the WDM transmission systems. When measuring the characteristics of such devices, wavelength tuneable laser sources are commonly used and are required to have well-calibrated performances; wavelength uncertainty, wavelength tuning repeatability, wavelength stability, and output optical power stability are important parameters.

The tuneable laser source (TLS) is generally equipped with the following features:

- a) the output wavelength is continuously tuneable in a wavelength range starting at 1 260 nm or higher and ending at less than 1 675 nm (the output should excite only the fundamental LP01 fibre mode);
- b) an output port for optical fibre connectors.

The envelope of the spectrum is a single longitudinal mode with a full-width at half-maximum (FWHM) of at most 0,1 nm. Any adjacent modes are at least 20 dB lower than the main spectral mode (for example, a distributed feedback laser diode (DFB-LD), external cavity laser, etc.).

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## CALIBRATION OF TUNEABLE LASER SOURCES

### 1 Scope

This document provides a stable and reproducible procedure to calibrate the wavelength and power output of a tuneable laser against reference instrumentation such as optical power meters and optical wavelength meters (including optical frequency meters) that have been previously traceably calibrated.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60793-2-50, *Optical fibres – Part 2-50: Product specifications – Sectional specification for class B single-mode fibres*

IEC 60825-1, *Safety of laser products – Part 1: Equipment classification and requirements*

IEC 60825-2, *Safety of laser products – Part 2: Safety of optical fibre communication systems (OFCSS)*

IEC 61315, *Calibration of fibre-optic power meters*

IEC 62129-2, *Calibration of wavelength/optical frequency measurement instruments – Part 2: Michelson interferometer single wavelength meters*

ISO/IEC Guide 98-3:2008, *Uncertainty of measurement – Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

### 3 Terms, definitions, and abbreviated terms

#### 3.1 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- IEC Electropedia: available at <https://www.electropedia.org/>
- ISO Online browsing platform: available at <https://www.iso.org/obp>

##### 3.1.1

##### **accredited calibration laboratory**

calibration laboratory authorized by an appropriate national organization to issue calibration certificates that demonstrates traceability to national standards

### 3.1.2

#### **adjustment**

set of operations carried out on an instrument in order that it provides given indications corresponding to given values of the measurand

Note 1 to entry: For more information, see ISO/IEC Guide 99:2007, 3.11.

[SOURCE: IEC 60050-311:2001, 311-03-16, modified – Domain deleted, words "measuring instrument" deleted in the definition, and omission of the Note to entry therein.]

### 3.1.3

#### **calibration**

set of operations that establish, under specified conditions, the relationship between the values of quantities indicated by a measuring instrument and the corresponding values realized by standards

Note 1 to entry: The results of a calibration permit either the assignment of measurand values to the indications or the determination of corrections with respect to the indications.

Note 2 to entry: A calibration can also determine other metrological properties such as the effects of influence quantities.

Note 3 to entry: The result of a calibration can be recorded in a document, called a calibration certificate or a calibration report.

Note 4 to entry: See also ISO/IEC Guide 99:2007, 2.39.

### 3.1.4

#### **calibration conditions**

conditions of measurement in which the calibration is performed

### 3.1.5

#### **calibration at reference conditions**

calibration which includes the evaluation of the uncertainty at reference conditions of the light source under calibration

### 3.1.6

#### **calibration at operating conditions**

calibration which includes the evaluation of the uncertainty at operating conditions of the light source under calibration

### 3.1.7

#### **level of confidence**

estimated probability that the true value of a measured parameter lies in the given range

### 3.1.8

#### **coverage factor**

$k$

factor used to calculate the expanded uncertainty  $U$  from the standard uncertainty  $u$

**3.1.9****optical power deviation** $D_P$ 

difference between the set power of the light source under calibration,  $P_{\text{TLS}}$ , and the corresponding reference power,  $P_{\text{meas}}$ , measured by the reference power meter

$$D_P = \frac{P_{\text{TLS}} - P_{\text{meas}}}{P_{\text{meas}}}$$

Note 1 to entry: Power  $P$  is expressed in linear units, for example W.

Note 2 to entry: This deviation is relative, it has no unit (it can be expressed in %).

**3.1.10****operating conditions**

appropriate set of specified ranges of values with influence quantities usually wider than the reference conditions for which the uncertainties of a measuring instrument are specified

Note 1 to entry: Operating conditions and the uncertainty at operating conditions are usually specified by the manufacturer for the convenience of the user.

**3.1.11****reference conditions**

conditions used for testing the performance of a measuring instrument or for the intercomparison of the measurement results

Note 1 to entry: Reference conditions generally include reference values or reference ranges for the quantities influencing and affecting the measuring instrument.

**3.1.12****side-mode suppression ratio**

SMSR

peak power ratio between the main-mode spectrum and the largest side mode spectrum in a single-mode laser diode such as a DFB-LD

Note 1 to entry: Side-mode suppression ratio is usually expressed in dB.

**3.1.13****wavelength**

wavelength (in a vacuum) of a light source

**3.1.14****wavelength deviation** $D_\lambda$ 

difference between the target wavelength, set on the light source under calibration,  $\lambda_{\text{TLS}}$ , and the measured wavelength,  $\lambda_{\text{meas}}$ , in nm or  $\mu\text{m}$

$$D_\lambda = \lambda_{\text{TLS}} - \lambda_{\text{meas}}$$

### 3.2 Abbreviated terms

|        |                                  |
|--------|----------------------------------|
| APC    | angled physical contact          |
| AWG    | arrayed waveguide grating        |
| DFB-LD | distributed feedback laser diode |
| DMUX   | demultiplexers                   |
| FWHM   | full-width at half-maximum       |
| MUX    | multiplexers                     |
| O/E    | optical-electrical               |
| OSA    | optical spectrum analyser        |
| RIN    | relative intensity noise         |
| SMSR   | side-mode suppression ratio      |
| TLS    | tuneable laser source            |
| WDM    | wavelength-division multiplexing |

## 4 Preparation for calibration

### 4.1 Organization

The calibration laboratory should ensure that suitable requirements for calibration are followed.

NOTE Guidance about good practices for calibration can be found in ISO/IEC 17025.

There should be a documented measurement procedure for each type of calibration performed, giving step-by-step operating instructions and equipment to be used.

### 4.2 Traceability

The calibration laboratory should ensure that suitable requirements are followed.

NOTE Guidance about good practices for calibration can be found in ISO/IEC 17025.

All standards used in the calibration process shall be calibrated according to a documented program with traceability to national standards laboratories or to accredited calibration laboratories.

It is advisable to maintain more than one standard on each hierarchical level, so that the performance of the standard can be verified by comparisons on the same level. Make sure that any other calibration equipment which have a significant influence on the calibration results are calibrated.

### 4.3 Preparation

The environmental conditions shall be commensurate with the level of uncertainty that is required for calibration:

- calibrations shall be carried out in a clean environment;
- temperature monitoring and control is required;
- all laser sources shall be safely operated (according to IEC 60825-1 and IEC 60825-2);
- the output of the TLS should be examined with an optical spectrum analyser (OSA) having sufficient resolution to resolve the longitudinal mode structure to check for single mode operation.

The recommended temperature is 23 °C, for example,  $(23 \pm 2)$  °C. Give the calibration equipment enough time prior to testing (2 h is recommended) to reach equilibrium within its environment. Allow the TLS a warm-up period in accordance with the manufacturer's instructions.

#### 4.4 Reference calibration conditions

The reference calibration conditions usually include the following parameters and, if necessary, their tolerance bands: date, temperature, relative humidity, atmospheric pressure, displayed optical power, displayed wavelength, fibre, connector-adapter combination, (spectral) bandwidth and resolution bandwidth (spectral resolution) set. Unless otherwise specified, use a single-mode optical fibre category B1.1 or B1.3 pigtail as specified in IEC 60793-2-50, having a length of at least 2 m. It is desirable to perform all the calibration in a situation where back-reflections are negligible. Thus, angled connectors and isolators should be used wherever the situation permits.

Operate the TLS in accordance with the manufacturer's specifications and operating procedures. Where practical, select a range of calibration conditions and parameters that emulate the actual field operating conditions of the TLS under calibration. Choose these parameters to optimize the tuneable laser source's accuracy, as specified by the manufacturer's operating procedures.

Document the conditions as specified in Clause 7.

NOTE The calibration results only apply to the set of calibration conditions used in the calibration process.

## 5 Wavelength calibration

### 5.1 Overview

The factors making up the uncertainty in the wavelength of the light source under calibration consist of:

- the intrinsic uncertainty of the light source under calibration as found in the calibration at reference conditions, including temperature and time dependences for these tight conditions, and;
- the uncertainties due to dependences on optical power, temperature and time as found in the calibrations at broader operating conditions.

The list of the source of uncertainty is summarized in Table 1.

**Table 1 – Source of uncertainty for wavelength calibration**


| Source of uncertainty        | Type of origin                 | Symbol                        |
|------------------------------|--------------------------------|-------------------------------|
| Repeatability                | Measurement                    | $s_{\lambda_j}$               |
| Temperature                  | Environment                    | $u_{\lambda_j, \Delta\Theta}$ |
| Stability                    | Light source under calibration | $u_{\lambda_j, \Delta t}$     |
| Wavelength resolution        | Reference wavelength meter     | $u_{\lambda_j, \text{res}}$   |
| Wavelength meter calibration | Reference wavelength meter     | $u_{\text{WM}, \lambda_j}$    |
| Optical power                | Light source under calibration | $u_{\lambda_j, P}$            |

The wavelength calibration at reference conditions for discrete wavelengths, as described in 5.2, is mandatory. The calibration at operating conditions, described in 5.3, is optional.

## 5.2 Wavelength calibration at reference conditions

### 5.2.1 Set-up

Figure 1 shows a system for wavelength calibration. The calibration is performed under the given reference conditions.

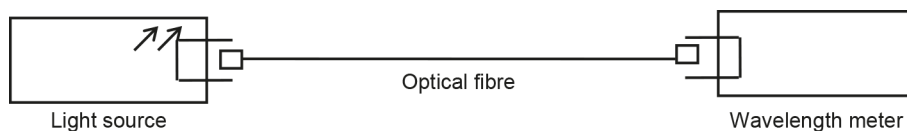

**Figure 1 – Measurement set-up for wavelength calibration**

### 5.2.2 Calibration equipment

A wavelength meter shall be used for the calibration. The wavelength meter shall be calibrated according to IEC 62129-2.

### 5.2.3 Procedure for wavelength calibration

The calibration procedure is as follows:

- Regarding the calibration system shown in Figure 1, the set wavelength of the light source is given by  $\lambda_{\text{TLS } j}$  and the measured values are given by  $\lambda_{\text{meas } i, j}$ . The uncertainty of the wavelength measurement takes into account the tuning repeatability and hysteresis of the TLS. Hysteresis is defined as the deviation resulting from tuning the desired wavelength from both the shorter and the longer wavelengths.
- It is recommended to repeat the wavelength measurement ten ( $m$ ) times. Ensure that the TLS is tuned to  $\lambda_{\text{TLS } j}$  prior to each measurement. The target wavelength ( $j$ ) should be approached in such a way that tuning occurs from both longer and shorter wavelengths.
- Calculate the average measured wavelength  $\bar{\lambda}_{\text{meas } j}$ :

$$\bar{\lambda}_{\text{meas}, j} = \frac{1}{m} \sum_{i=1}^m \lambda_{\text{meas } i, j} \quad (1)$$

where

$m$  is the number of measurements performed.

Each  $\lambda_{\text{meas } i, j}$  is suggested to be an averaged value from the wavelength meter.

- Calculate the wavelength deviation  $D_{\lambda_j}$ :

$$D_{\lambda_j} = \lambda_{\text{TLS } j} - \bar{\lambda}_{\text{meas } j} \quad (2)$$

where  $\lambda_{\text{TLS } j}$  is the tuned wavelength of the TLS.

- e) Calculate the standard deviation for  $\lambda_j$  from the ( $m$ ) wavelength measurement results  $\lambda_{\text{meas } i, j}$ :

$$s_{\lambda_j} = \left[ \frac{1}{m-1} \sum_{i=1}^m (\lambda_{\text{meas } i, j} - \bar{\lambda}_{\text{meas } j})^2 \right]^{\frac{1}{2}} \quad (3)$$

- f) Calculate the wavelength tuning repeatability  $S_{\text{rep}, \lambda_j}$ :

$$S_{\text{rep}, \lambda_j} = 2 \times s_{\lambda_j} \quad (4)$$

NOTE A default level of confidence of 95 % is used in Formula (4).


This calibration procedure shall be performed for each calibration wavelength. A minimum of 10 discrete wavelengths or every 10 nm, including the first, the central and the last wavelength of the range, shall be measured.

## 5.2.4 Dependence on conditions

### 5.2.4.1 Temperature dependence (optional if known)

#### 5.2.4.1.1 Set-up

Figure 2 shows a calibration system for temperature dependence. This calibration is performed under the reference calibration conditions with the exception of temperature.

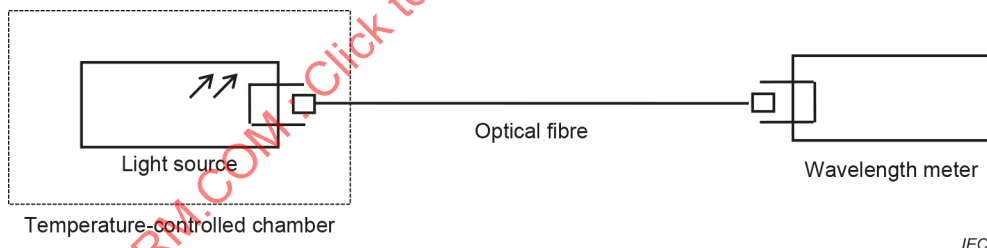

**Figure 2 – Measurement set-up for temperature dependence**

#### 5.2.4.1.2 Calibration equipment

The calibration equipment is as follows:

- A wavelength meter capable of detecting wavelength deviation of the TLS due to temperature.
- Temperature-controlled chamber: make sure that the measurement results are immune to the inner temperature distribution.

#### 5.2.4.1.3 Calibration procedure for determining temperature dependence

The calibration procedure is as follows:

- Regarding the calibration system of Figure 2, measure the nominal wavelength ( $j$ ) of the TLS at optical power  $P_{\text{TLS } j}$  at reference conditions:  $\lambda_{j, \text{ref}}$ . The wavelength used should possess the maximum response to temperature variations. Otherwise, characterization of several output wavelengths should be performed.

- b) Measure the wavelength of the TLS at temperature ( $i$ ):  $\lambda_{j,\Theta_i}$ . Wavelength readings corresponding to each temperature setting should be averaged to determine  $\lambda_{j,\Theta_i}$ .
- c) Calculate the wavelength deviation:

$$D_{\lambda_{j,\Theta_i}} = \lambda_{j,\Theta_i} - \lambda_{j,\text{ref}} \quad (5)$$

- d) Repeat steps b) and c) with ( $m$ ) different temperature settings  $\Theta_i$  ensuring that the instrument is allowed the necessary time to eliminate sufficiently any thermal gradients.
- e) Calculate the maximum  $\max(D_{\lambda_{j,\Theta_i}})_{i=1}^{i=m}$  and minimum  $\min(D_{\lambda_{j,\Theta_i}})_{i=1}^{i=m}$  wavelength deviations.
- f) The standard uncertainty for wavelength temperature dependence  $u_{\lambda_{j,\Delta\Theta}}$  at the calibration wavelength ( $j$ ) using a rectangular distribution model is:

$$u_{\lambda_{j,\Delta\Theta}} = \frac{1}{2\sqrt{3}} \left[ \max(D_{\lambda_{j,\Theta_i}})_{i=1}^{i=m} - \min(D_{\lambda_{j,\Theta_i}})_{i=1}^{i=m} \right] \quad (6)$$

where


$\Delta\Theta$  is the temperature variation.

It is recommended that a wavelength acquisition be performed with the optical wavelength meter for the duration of this calibration.

#### 5.2.4.2 Wavelength stability

##### 5.2.4.2.1 Set-up

Figure 3 shows a calibration system for wavelength stability. This calibration is performed under the reference calibration conditions with the exception of time.

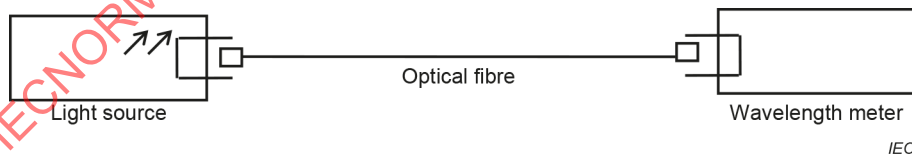

**Figure 3 – Measurement set-up for wavelength stability**

##### 5.2.4.2.2 Calibration equipment

It is recommended to use a wavelength meter capable of detecting wavelength fluctuations of the TLS.

### 5.2.4.2.3 Calibration procedure for wavelength stability

The calibration procedure is as follows:

- A time period ( $\Delta t$ ), for example 10 min, shall be chosen that is long enough to permit at least 10 wavelength measurements with the reference wavelength meter (in the case of the example, a stability over 10 min will be measured).
- A continuous wavelength acquisition should be performed with wavelength data and time stamp.
- Ensure to correlate ( $m$ ) measurements per time period where ( $m > 10$ ) and conforms exactly to the desired time period ( $\Delta t$ ).
- Calculate the standard deviation of the ( $m$ ) wavelength measurements corresponding to time period ( $\Delta t$ )

$$u_{\lambda_j, \Delta t} = \left[ \frac{1}{m-1} \sum_{i=1}^m (\lambda_{j, t_i} - \frac{1}{m} \sum_{i=1}^m \lambda_{j, t_i})^2 \right]^{\frac{1}{2}} \quad (7)$$

- A minimum of 1 time period is required to evaluate the wavelength stability of the TLS source. In this case, the wavelength stability uncertainty becomes:

$$S_{\text{stab}, \lambda_j, \Delta t} = 2 \times u_{\lambda_j, \Delta t} \quad (8)$$

NOTE A default level of confidence of 95 % is used in Formula (8).

The wavelength of the light source should be measured more than ten times ( $m$  times) consecutively; at least a few measurements per minute is recommended. The time interval between the repeated measurements should be longer than the response time of the light source. It is preferred to calculate several time periods from the acquisition data using a sliding window and report the maximum value.

### 5.2.5 Uncertainty at reference conditions

The uncertainty for the calibration wavelength ( $j$ ) at reference conditions is given by:

$$u_{\lambda_j, \text{ref}} = \left( \frac{s_{\lambda_j}^2}{m} + u_{\lambda_j, \Delta \Theta}^2 + u_{\lambda_j, \Delta t}^2 + u_{\lambda_j, \text{res}}^2 + u_{\text{WM}_{\lambda_j}}^2 \right)^{\frac{1}{2}} \quad (9)$$

where

$u_{\lambda_j, \Delta \Theta}$  and  $u_{\lambda_j, \Delta t}$  are evaluated for the reference conditions as defined in 5.2.4;

$u_{\lambda_j, \text{res}}$  is the uncertainty of wavelength resolution defined by  $u_{\lambda_j, \text{res}} = d\lambda_j / 2\sqrt{3}$  ( $d\lambda_j$  is the wavelength resolution of the wavelength meter);

$u_{\text{WM}_{\lambda_j}}$  is the uncertainty of the wavelength meter at wavelength ( $j$ ) as described in its certification.

The expanded uncertainty for the calibration wavelength ( $\lambda$ ) at reference conditions,  $U_{\lambda_{j,\text{ref}}}$ , with a coverage factor  $k$  is expressed as follows:

$$U_{\lambda_{j,\text{ref}}} = k u_{\lambda_{j,\text{ref}}} \quad (10)$$

where

$k$  corresponds to an appropriate level of confidence as described in Clause A.5.

Refer to Annex A and Annex C for information on uncertainties.

When adjustments are made to the instrument based on the calibration results, it is advisable to repeat the calibrations after these adjustments to verify the corrections.

### 5.3 Wavelength calibration at operating conditions

#### 5.3.1 General

Perform the calibration procedure when the light source is used beyond the reference conditions.


The individual factors in wavelength uncertainty at operating conditions consist of following:

- a) optical power dependence;
- b) temperature dependence;
- c) wavelength stability.

#### 5.3.2 Optical power dependence

##### 5.3.2.1 General

Figure 4 shows a calibration system for optical power dependence. This calibration should be performed under the reference calibration conditions with the exception of the optical power. It shall be performed after the optical power calibration (6.2.3).

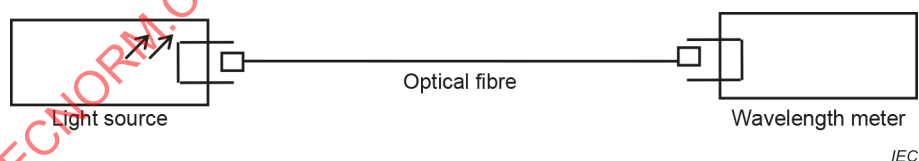

**Figure 4 – Measurement set-up for optical power dependence**

##### 5.3.2.2 Calibration equipment

The wavelength meter shall be calibrated according to IEC 62129-2.

### 5.3.2.3 Calibration procedures for determining power dependence

The calibration procedures are as follows:

- The wavelength ( $j$ ) is measured at  $m$  optical powers of the light source,  $P_{\text{TLS } i,j}$  including the upper and lower limits of the specified power range. The interval between these neighbouring levels should be smaller than 10 dB.
- Regarding the calibration system of Figure 4, the set wavelength of the light source is given by  $\lambda_{\text{TLS } i,j}$ , and the instrument reading of the wavelength meter is given by  $\lambda_{P_{i,j}}$ .
- Record the measured wavelength  $\lambda_{P_{i,j}}$  for all ( $m$ ) output power settings  $P_{\text{TLS } i,j}$  used.
- Calculate the standard uncertainty of wavelength ( $j$ ) due to TLS output optical power according to

$$u_{\lambda_j, P} = \left[ \frac{1}{m-1} \sum_{i=1}^m (\lambda_{P_{i,j}} - \frac{1}{m} \sum_{i=1}^m \lambda_{P_{i,j}})^2 \right]^{\frac{1}{2}} \quad (11)$$

### 5.3.3 Uncertainty at operating conditions

The uncertainty for the calibration wavelength ( $j$ ) for any operating conditions is given by

$$u_{\lambda_j, \text{op}} = \left( s_{\lambda_j}^2 + u_{\lambda_j, P}^2 + u_{\lambda_j, \Delta\Theta}^2 + u_{\lambda_j, \Delta t}^2 + u_{\lambda_j, \text{res}}^2 + u_{\text{WM}_{\lambda_j}}^2 \right)^{\frac{1}{2}} \quad (12)$$

where

$u_{\lambda_j, P}$ ,  $u_{\lambda_j, \Delta\Theta}$  and  $u_{\lambda_j, \Delta t}$  are evaluated for the operating conditions;

$u_{\lambda_j, \text{res}}$  is the uncertainty of wavelength resolution defined by  $u_{\lambda_j, \text{res}} = d\lambda_j / 2\sqrt{3}$  ( $d\lambda_j$  is wavelength resolution of the wavelength meter);

$u_{\text{WM}_{\lambda_j}}$  is the uncertainty of the wavelength meter at wavelength ( $j$ ) as described in its certification.

The expanded uncertainty for the calibration wavelength ( $j$ ) under all operating conditions,  $U_{\lambda_j, \text{op}}$ , with a coverage factor  $k$ , is expressed as follows:

$$U_{\lambda_j, \text{op}} = k u_{\lambda_j, \text{op}} \quad (13)$$

where

$k$  corresponds to an appropriate level of confidence as described in Clause A.5.

## 6 Optical power calibration

### 6.1 Overview

The factors making up the uncertainty in the set optical power of the light source under calibration consists of

- the intrinsic uncertainty of the light source under calibration as found in the calibration at reference conditions including temperature, time, and connection repeatability/reproducibility dependences for these tight conditions, and
- the uncertainties due to dependences on wavelength, temperature, time and connection repeatability/reproducibility, as found in the calibrations at broader operating conditions.

The list of the source of uncertainty is summarized in Table 2.

**Table 2 – Source of uncertainty for optical power calibration**


| Source of uncertainty           | Type of origin                 | Symbol                   |
|---------------------------------|--------------------------------|--------------------------|
| Repeatability                   | Measurement                    | $s_{DP_j}$               |
| Temperature                     | Environment                    | $u_{DP_j, \Delta\Theta}$ |
| Stability                       | Light source under calibration | $u_{DP_j, \Delta t}$     |
| Connection reproducibility      | Light source under calibration | $u_{DP_j, \text{con}}$   |
| Optical power resolution        | Reference optical power meter  | $u_{DP_j, \text{res}}$   |
| Optical power meter calibration | Reference optical power meter  | $u_{PM_{P_j}}$           |
| Wavelength                      | Light source under calibration | $u_{DP_j, \lambda}$      |

The optical power calibration at reference conditions as described in 6.2 is mandatory. The calibration at operating conditions described in 6.3 is optional.

### 6.2 Optical power calibration at reference conditions

#### 6.2.1 Set-up

Figure 5 shows a system for the calibration of the optical power. The calibration is performed under the given reference conditions.

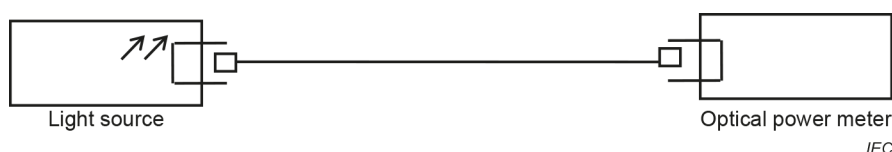

**Figure 5 – Measurement set-up for intrinsic optical power calibration**

NOTE There could be problems in calibrating the power of a highly coherent laser source, due to parasitic interference effects arising from reflections from fibre connector end faces and also the optical power meter. The use of angled physical contact (APC) connectors, inline optical isolators and engaging of the laser's coherent control function (if fitted) can reduce the interference effects to an acceptable level.

The optical power to be calibrated is measured at the end of an optical fibre cable, which can cause some insertion losses. The calibration condition about the used optical fibre cable such as fibre length, connector type, inline isolator if any, should be reported.

### 6.2.2 Calibration equipment

The optical power meter shall be calibrated according to IEC 61315.

### 6.2.3 Procedure for power calibration at reference conditions

The calibration procedure is as follows:

- Connect the light source and the power meter with the optical fibre.
- Set the wavelength of the light source and the optical power meter to the required calibration wavelength.
- Set the output power of the light source to  $P_{\text{TLS}j}$ . The uncertainty of the power measurement takes into account the setting repeatability and hysteresis of the TLS. Hysteresis is defined as the deviation resulting from setting the desired power from both the lower and the higher powers.
- Read the measured value of optical power meter.
- It is recommended to repeat this measurement ten ( $m$ ) times. Ensure that the TLS is set to  $P_{\text{TLS}j}$  prior to each measurement. The target power should be approached in such a way that setting occurs from both lower and higher powers.

$$D_{P_{i,j}} = \frac{P_{\text{TLS}j} - P_{\text{meas } i,j}}{P_{\text{meas } i,j}} \quad (14)$$

where

$P_{\text{TLS}j}$  is the set optical power of the TLS.

Each  $P_{\text{meas } i,j}$  is suggested to be an averaged value from the power meter. Calculate the power deviation  $D_{P_j}$ .

$$D_{P_j} = \frac{1}{m} \sum_{i=1}^m D_{P_{i,j}} \quad (15)$$

where

$m$  is the number of measurements performed.

- Calculate the standard deviation for  $D_{P_j}$  from the ( $m$ ) power measurement results  $P_{\text{meas } i,j}$ :

$$s_{D_{P_j}} = \left[ \frac{1}{m-1} \sum_{i=1}^m (D_{P_{i,j}} - D_{P_j})^2 \right]^{\frac{1}{2}} \quad (16)$$

g) Calculate the optical power setting repeatability:  $S_{\text{rep},DP_j}$

$$S_{\text{rep},DP_j} = 2 \times s_{DP_j} \quad (17)$$

NOTE A default level of confidence of 95 % is used in Formula (17).


The uncertainty calculations (6.2.3 a) to g)) should be performed for each calibration power.

## 6.2.4 Dependence on conditions

### 6.2.4.1 Temperature dependence (optional if known)

#### 6.2.4.1.1 Set-up

Figure 6 shows a calibration system for temperature dependence. This calibration is performed under the reference calibration conditions with the exception of temperature.

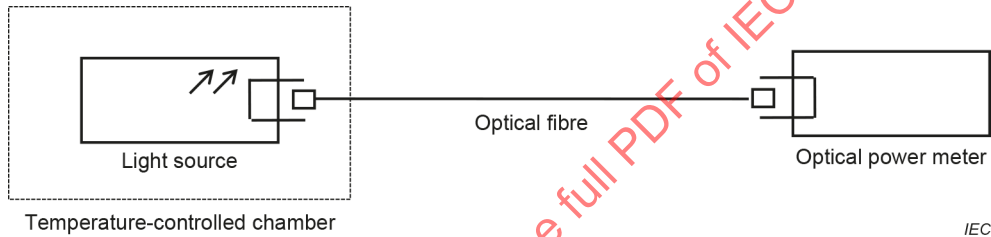

**Figure 6 – Measurement set-up for temperature dependence**

#### 6.2.4.1.2 Calibration equipment

The calibration equipment is as follows:

- An optical meter capable of detecting optical power deviation of the TLS depending on temperature.
- Temperature-controlled chamber:  
Make sure that the measurement results are immune to the inner temperature distribution.

#### 6.2.4.1.3 Calibration procedure for determining temperature dependence

The calibration procedure is as follows:

- Regarding the calibration system of Figure 6, measure the nominal optical power of the TLS at wavelength  $\lambda_{\text{TLS}j}$  at reference conditions  $P_{j,\text{ref}}$ . The optical power used should possess the maximum response to temperature variations. Otherwise, characterization of several output optical powers will be required.
- Measure the optical power of the TLS at temperature ( $i$ ):  $P_{j,\Theta_i}$ . Optical power readings corresponding to each temperature setting should be averaged to determine  $P_{j,\Theta_i}$ .
- Calculate the relative optical power deviation:

$$DP_{j,\Theta_i} = \frac{P_{j,\Theta_i} - P_{j,\text{ref}}}{P_{j,\text{ref}}} \quad (18)$$

- d) Repeat steps b) and c) with  $(m)$  different temperature settings  $\Theta_i$  ensuring that the instrument is allowed the necessary time to eliminate sufficiently any thermal gradients.
- e) Calculate the maximum  $\max(D_{P_j, \Theta_i})_{i=1}^{i=m}$  and minimum  $\min(D_{P_j, \Theta_i})_{i=1}^{i=m}$  optical power deviations.
- f) The standard uncertainty for optical power temperature dependence  $u_{P_j, \Delta\Theta}$  at the calibration optical power using a rectangular distribution model is:

$$u_{D_{P_j, \Delta\Theta}} = \frac{1}{2\sqrt{3}} \left[ \max(D_{P_j, \Theta_i})_{i=1}^{i=m} - \min(D_{P_j, \Theta_i})_{i=1}^{i=m} \right] \quad (19)$$

where


$\Delta\Theta$  is the temperature variation.

It is recommended that a optical power acquisition be performed with the optical power meter for the duration of this calibration.

#### 6.2.4.2 Optical power stability

##### 6.2.4.2.1 Set-up

Figure 7 shows a calibration system for optical power stability. This calibration is performed under the reference calibration conditions with the exception of time.

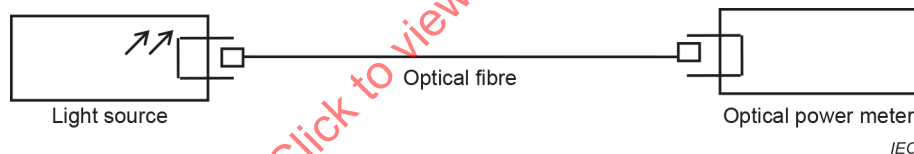

**Figure 7 – Measurement set-up for optical power stability**

##### 6.2.4.2.2 Calibration equipment

It is recommended to use an optical power meter capable of detecting optical power fluctuations of the TLS.

##### 6.2.4.2.3 Calibration procedure for optical power stability

The calibration procedure is as follows:

- a) A specific time period ( $\Delta t$ ), for example 10 min, shall be chosen that is long enough to permit at least 10 optical power measurements with the reference power meter (in the case of the example, a stability over 10 min will be measured).
- b) A continuous optical power acquisition should be performed with optical power data and time stamp.
- c) Ensure to correlate  $(m)$  measurements per time period where  $(m > 10)$  and conforms exactly to the desired time period ( $\Delta t$ ).

d) Calculate the standard deviation of the ( $m$ ) measurements corresponding to time period ( $\Delta t$ ):

$$u_{D_{P_j, \Delta t}} = \left[ \frac{1}{m-1} \sum_{i=1}^m (P_{j, t_i} - \frac{1}{m} \sum_{i=1}^m P_{j, t_i})^2 \right]^{\frac{1}{2}} / \left( \frac{1}{m} \sum_{i=1}^m P_{j, t_i} \right) \quad (20)$$

e) A minimum of 1 time period is required to evaluate the optical power stability of the TLS source. In this case, the optical power stability uncertainty becomes:

$$S_{\text{stab}, D_{P_j, \Delta t}} = 2 \times u_{D_{P_j, \Delta t}} \quad (21)$$

NOTE A default level of confidence of 95 % is used in Formula (21).


It is preferred to calculate several time periods from the acquisition data using a sliding window and report the maximum value.

The optical power of the light source should be measured more than ten times ( $m$  times) consecutively; at least a few measurements per minute is recommended. The time interval between the repeated measurements should be longer than the response time of the light source.

#### 6.2.4.3 Connection repeatability/reproducibility

##### 6.2.4.3.1 Set-up

Figure 8 shows a calibration system for optical power stability. This calibration is performed under the reference calibration conditions.

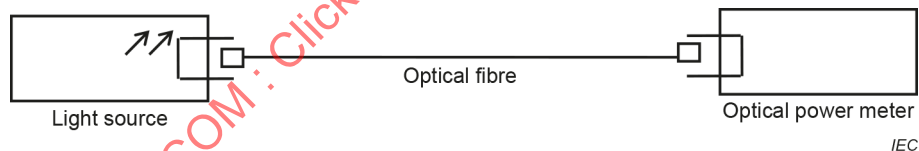

**Figure 8 – Measurement set-up for connection repeatability/reproducibility**

##### 6.2.4.3.2 Calibration equipment

The optical power meter shall be calibrated according to IEC 61315.

##### 6.2.4.3.3 Calibration procedure for connection repeatability/reproducibility

The calibration procedure is as follows:

- Regarding the calibration system in Figure 8, connect the light source and the power meter with the optical fibre.
- Read the measured value of optical power meter  $P_{j, \text{con}_i}$ .
- Disconnect the optical fibre from the TLS and reconnect the optical fibre to the TLS.
- Repeat b) and c) for ( $m$ ) times.

- e) Calculate the standard uncertainty of optical power ( $j$ ) due to TLS connection repeatability/reproducibility according to

$$u_{D_{P_j, \text{con}}} = \left[ \frac{1}{m-1} \sum_{i=1}^m \left( P_{j, \text{con}_i} - \frac{1}{m} \sum_{i=1}^m P_{j, \text{con}_i} \right)^2 \right]^{\frac{1}{2}} / \left( \frac{1}{m} \sum_{i=1}^m P_{j, \text{con}_i} \right) \quad (22)$$

### 6.2.5 Uncertainty at reference conditions

The uncertainty for the calibration optical power at reference conditions is given by:

$$u_{D_{P_j, \text{ref}}} = \left( \frac{s_{D_{P_j}}^2}{m} + u_{D_{P_j, \Delta\Theta}}^2 + u_{D_{P_j, \Delta t}}^2 + u_{D_{P_j, \text{con}}}^2 + u_{D_{P_j, \text{res}}}^2 + u_{\text{PM}_{P_j}}^2 \right)^{\frac{1}{2}} \quad (23)$$

where

$u_{D_{P_j, \Delta\Theta}}$ ,  $u_{D_{P_j, \Delta t}}$  and  $u_{D_{P_j, \text{con}}}$  are evaluated for the reference conditions as defined in 6.2.4;

$u_{D_{P_j, \text{res}}}$  is the relative uncertainty of optical power resolution defined by

$u_{D_{P_j, \text{res}}} = (dP_{\text{TLS}, j} / P_{\text{TLS}, j}) / 2\sqrt{3}$  ( $dP_{\text{TLS}, j}$  is the optical power resolution of the optical power meter);

$u_{\text{PM}_{P_j}}$  is the relative uncertainty of the power meter at power  $P_j$  as described in its certification.

The expanded uncertainty for the calibration power meter at reference conditions  $U_{D_{P_j, \text{ref}}}$ , with a coverage factor  $k$ , is expressed as follows:

$$U_{D_{P_j, \text{ref}}} = k u_{D_{P_j, \text{ref}}} \quad (24)$$

where

$k$  corresponds to an appropriate level of confidence as described in Clause A.5.

Refer to Annex A for information on uncertainties.

When adjustments are made to the instrument based on the calibration results, it is advisable to repeat the calibrations after these adjustments to verify the corrections.

## 6.3 Optical power calibration at operating conditions

### 6.3.1 General

Perform the calibration procedure when the light source is used beyond the reference conditions.


The individual factors in optical power uncertainty at operating conditions consist of the following:

- a) wavelength dependence;
- b) temperature dependence;
- c) optical power stability;
- d) connection repeatability/reproducibility.

### 6.3.2 Wavelength dependence

#### 6.3.2.1 Set-up

Figure 9 shows a calibration system for wavelength dependence. This calibration should be performed under the reference calibration conditions with the exception of the wavelength. It shall be performed after the wavelength calibration (5.2.3).

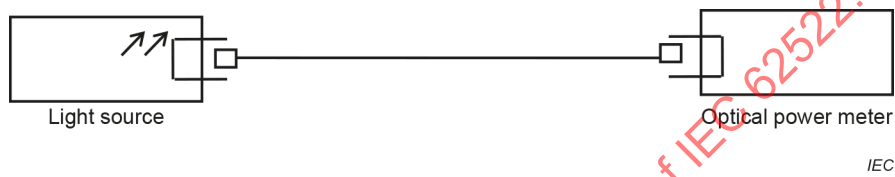

**Figure 9 – Measurement set-up for wavelength dependence**

#### 6.3.2.2 Calibration equipment

The calibration equipment is as follows: the optical power meter should be calibrated according to IEC 61315.

#### 6.3.2.3 Calibration procedure for determining wavelength dependence

The calibration procedure is as follows:

- a) The optical power is measured at  $m$  wavelengths (more than 5) of the light source,  $\lambda_{\text{TLS } i,j}$  including the upper and lower limits of the specified wavelength range.
- b) Regarding the calibration system of Figure 9, the set optical power of the light source is given by  $P_{\text{TLS } i,j}$ , and the instrument reading of the power meter is given by  $P_{\lambda_{i,j}}$ .
- c) Set the wavelength of the optical power meter to the required calibration wavelength.
- d) Record the measured optical power  $P_{\lambda_{i,j}}$  for all ( $m$ ) wavelength settings  $\lambda_{\text{TLS } i,j}$  used.
- e) Calculate the standard uncertainty of optical power ( $j$ ) due to TLS output wavelength according to:

$$u_{D_{P_j, \lambda}} = \left[ \frac{1}{m-1} \sum_{i=1}^m \left( P_{\lambda_{i,j}} - \frac{1}{m} \sum_{i=1}^m P_{\lambda_{i,j}} \right)^2 \right]^{\frac{1}{2}} / \left( \frac{1}{m} \sum_{i=1}^m P_{\lambda_{i,j}} \right) \quad (25)$$

### 6.3.3 Uncertainty at operating conditions

The uncertainty for the calibration optical power for any operating condition is given by:

$$u_{D_{P_j,op}} = \left( s_{D_{P_j}}^2 + u_{D_{P_j,\lambda}}^2 + u_{D_{P_j,\Delta\theta}}^2 + u_{D_{P_j,\Delta t}}^2 + u_{D_{P_j,con}}^2 + u_{D_{P_j,res}}^2 + u_{PM_{P_j}}^2 \right)^{\frac{1}{2}} \quad (26)$$

where

$u_{D_{P_j,\lambda}}$ ,  $u_{D_{P_j,\Delta\theta}}$ ,  $u_{D_{P_j,\Delta t}}$  and  $u_{D_{P_j,con}}$  are evaluated for the operating conditions;

$u_{D_{P_j,res}}$  is the relative uncertainty of optical power resolution defined by  $u_{D_{P_j,res}} = (dP_{TLS,j} / P_{TLS,j}) / 2\sqrt{3}$  ( $dP_{TLS,j}$  is optical power resolution of the optical power meter);

$u_{PM_{P_j}}$  is the uncertainty of the power meter at optical power  $P_j$  as described in its certification.

The expanded uncertainty for the calibration optical power under all operating conditions  $U_{D_{P_j,op}}$ , with a coverage factor  $k$ , is expressed as follows:

$$U_{D_{P_j,op}} = k u_{D_{P_j,op}} \quad (27)$$

where

$k$  corresponds to an appropriate level of confidence as described in Clause A.5.

## 7 Documentation

### 7.1 Calibration data and uncertainty

Calibration certificates claiming to be in compliance with this document shall include the following data and their uncertainties, and the uncertainties shall be stated in the form of estimated confidence intervals by multiplying the relevant standard uncertainty by  $k$ :

NOTE 1 Refer to Annex A for information on uncertainty and Clause A.5 for further details on level of confidence and coverage factor.

- a) the wavelength deviation,  $D_{\lambda_j}$ , and its uncertainty,  $ku_{\lambda_j,ref}$ , for example, is in nm, in a vacuum – see the detailed requirements in Clause 5;
- b) the optical power deviation,  $D_{P_j}$ , and its uncertainty,  $ku_{D_{P_j,ref}}$ , for example, is in % or dB – see the detailed requirements in Clause 6.

NOTE 2 Other tests can be added to the documentation, refer to Annex B for more information.

## 7.2 Calibration conditions

The calibration method(s) and the method(s) of obtaining the measurement results shall be stated.

Calibration conditions shall be reported. The most important parameters are the calibration date, the displayed optical power, the displayed wavelength, the temperature, the humidity and the atmospheric pressure.

NOTE The calibration results only apply to the set of calibration conditions used for the calibration process.

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## Annex A (normative)

### Mathematical basis for measurement uncertainty calculations

#### A.1 General

Annex A summarizes the form of evaluating, combining, and reporting the uncertainty of measurement. It is based on ISO/IEC Guide 98-3. Annex A shall be read in conjunction with ISO/IEC Guide 98-3 for additional information.

This document distinguishes between two types of evaluation of uncertainty of measurement. Type A is the method of evaluation of uncertainty by the statistical analysis of a series of measurements on the same measurand. Type B is the method of evaluation of uncertainty based on other knowledge.

#### A.2 Type A evaluation of uncertainty

The type A evaluation of standard uncertainty can be applied when several independent observations have been made for a quantity under the same conditions of measurement.

For a quantity  $X$  estimated from  $n$  independent repeated observations  $X_k$ , the arithmetic mean is:

$$\bar{X} = \frac{1}{n} \sum_{k=1}^n X_k \quad (\text{A.1})$$

This mean is used as the estimate of the quantity, that is  $x = \bar{X}$ . The experimental standard deviation of the observations is given by:

$$s(X) = \left[ \frac{1}{n-1} \sum_{k=1}^n (X_k - \bar{X})^2 \right]^{1/2} \quad (\text{A.2})$$

where

$\bar{X}$  is the arithmetic mean of the observed values;

$X_k$  are the measurement samples of a series of measurements;

$n$  is the number of measurements; it is assumed to be large, for example,  $n \geq 10$ .

The type A standard uncertainty  $u_{\text{typeA}}(x)$  associated with the estimate  $x$  is the experimental standard deviation of the mean.

$$u_{\text{typeA}}(x) = s(\bar{X}) = \frac{s(X)}{\sqrt{n}} \quad (\text{A.3})$$

### A.3 Type B evaluation of uncertainty

The type B evaluation of standard uncertainty is the method of evaluating the uncertainty by means other than the statistical analysis of a series of observations. It is evaluated by scientific judgement based on all available information on the variability of the quantity.

If the estimate  $x$  of a quantity  $X$  is taken from a manufacturer's specification, calibration certificate, handbook, or other source and its quoted uncertainty  $U(x)$  is stated to be a multiple  $k$  of a standard deviation, the standard uncertainty  $u(x)$  is simply the quoted value divided by the multiplier.

$$u(x) = U(x) / k \quad (\text{A.4})$$

If only upper and lower limit  $X_{\max}$  and  $X_{\min}$  can be estimated for the value of the quantity  $X$  (for example a manufacturer's specifications or a temperature range), a rectangular probability distribution is assumed, and the estimated value is:

$$x = \frac{1}{2}(X_{\max} + X_{\min}) \quad (\text{A.5})$$

and the standard uncertainty is:

$$u(x) = \frac{1}{2\sqrt{3}}(X_{\max} - X_{\min}) \quad (\text{A.6})$$

The contribution to the standard uncertainty associated with the output estimate  $y$  resulting from the standard uncertainty associated with the input estimate  $x$  is:

$$u(y) = c \times u(x) \quad (\text{A.7})$$

where

$c$  is the sensitivity coefficient associated with the input estimate  $x$ , which is the partial derivative of the model function  $y(x)$ , evaluated at the input estimate  $x$ .

$$c = \frac{\partial y}{\partial x} \quad (\text{A.8})$$

The sensitivity coefficient  $c$  describes the extent to which the output estimate  $y$  is influenced by variations of the input estimate  $x$ . It can be evaluated by Formula (A.8) or by using numerical methods, that is by calculating the change in the output estimate  $y$  due to a change in the input estimate  $x$  from a model function. Sometimes, it can be more appropriate to find the change in the output estimate  $y$  due to the change of  $x$  from an experiment.

#### A.4 Determining the combined standard uncertainty

The combined standard uncertainty is used to collect a number of individual uncertainties into a single number. The combined standard uncertainty is based on statistical independence of the individual uncertainties. It is calculated by root-sum-squaring all standard uncertainties obtained from type A and type B evaluation:

$$u_c(y) = \sqrt{\sum_{i=1}^n u_i^2(y)} \quad (\text{A.9})$$

where

$i$  is the current number of individual contribution;

$u_i(y)$  are the standard uncertainty contributions;

$n$  is the number of uncertainties.

NOTE It is acceptable to neglect uncertainty contributions to Formula (A.9) that are smaller than 1/10 of the largest contribution, because squaring them will reduce their significance to 1/100 of the largest contribution.

When the quantities above are to be used as the basis for further uncertainty computations, then the combined standard uncertainty,  $u_c$ , can be re-inserted into Formula (A.9). Despite its partially type A origin,  $u_c$  should be considered as describing an uncertainty of type B.

#### A.5 Reporting

In calibration reports and technical data sheets, combined standard uncertainties shall be reported in the form of expanded uncertainties, together with the applicable level of confidence. Correction factors or deviations shall be reported. The expanded uncertainty  $U$  is obtained by multiplying the standard uncertainty  $u_c(y)$  by a coverage factor  $k$ :

$$U = k \times u_c(y) \quad (\text{A.10})$$

For a level of confidence of approximately 95 %, the default level, then  $k = 2$ . If a level of confidence of approximately 99 % is chosen, then  $k = 3$ . The above values for  $k$  are valid under some conditions, see ISO/IEC Guide 98-3 (GUM); if these conditions are not met, larger coverage factors are to be used to reach these levels of confidence.

## Annex B (informative)

### Other testing


#### B.1 General

Annex B provides some details on other tests which are not mandatory but are related to the performance of tuneable laser sources.

#### B.2 Wavelength tuning resolution

##### B.2.1 Set-up

Figure B.1 shows the test set-up for a wavelength tuning resolution test under standard test conditions.

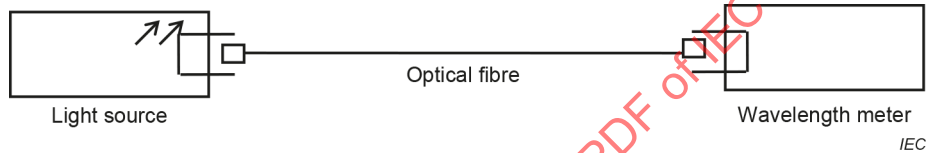

**Figure B.1 – Measurement set-up for wavelength resolution**

##### B.2.2 Testing equipment

Testing equipment is as follows:

A wavelength meter which has a better wavelength measurement resolution than the wavelength resolution of test light source should be used.

##### B.2.3 Testing procedure for determining wavelength resolution

The testing procedure is as follows:

- Set the wavelength of the test light source to  $\lambda_{\text{TLS}}$ . Set the optical output power of the test light source to a suitable value.
- The wavelength for  $\lambda_{\text{meas}}$  is measured with the wavelength meter.
- The wavelength of the light source is set only  $qd\lambda$  to the long (or short) wavelength side for  $\lambda_{\text{TLS}}$ . Here,  $d\lambda$  is the minimum variable width that can be set to  $\lambda_{\text{TLS}}$ , and  $q$  are integers.
- Inject the optical output of the light source into the wavelength meter. The wavelength for  $\lambda_{\text{meas}+1}$  is measured with the wavelength meter.
- After the wavelength of the light source is returned to  $\lambda_{\text{TLS}}$ , the measurements should be repeated over ten times ( $m$  times).
- Calculate the wavelength setting resolution  $d\lambda_{\text{TLS},j}$  with Formula (B.1).

$$d\lambda_{\text{TLS},j} = \sum_{i=1}^m \frac{|\lambda_{\text{meas}+1,i} - \lambda_{\text{meas},i}|}{m \times q} \quad (\text{B.1})$$


- g) Repeat the measurements for a few ( $j$ ) wavelengths covering the desired wavelength range. Calculate the wavelength setting resolution with Formula (B.2).

$$d\lambda_{\text{TLS}} = \max(d\lambda_{\text{TLS},j}) \quad (\text{B.2})$$

### B.3 Optical power tuning resolution

#### B.3.1 Set-up

Figure B.2 shows the test set-up for optical power tuning resolution setting tests under standard test conditions.

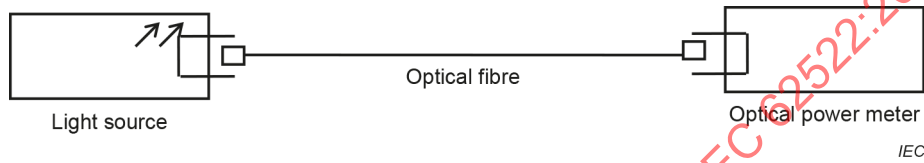

**Figure B.2 – Measurement set-up for optical power resolution setting test**

#### B.3.2 Testing equipment

Use an optical power meter with high resolution.

#### B.3.3 Testing procedure for optical power resolution

Testing procedure is as follows:

- Set the optical output power of the test light source to  $P_{\text{TLS}}$ . Set the wavelength of the light source to a suitable value.
- Inject the optical output into the optical power meter. Measure the optical power  $P_{\text{meas}}$  with the optical power meter.
- Only set the minimum variable width  $dP$  as a higher (or lower) output power under  $P_{\text{TLS}}$  settings for optical output power of test light source.
- Measure the optical power  $P_{\text{meas}+1}$  with optical power meter.
- After the optical output power of test light source is returned to  $P_{\text{TLS}}$ , the measurements should be repeated over ten times ( $m$  times).
- Calculate the optical output power setting resolution  $dP_{\text{TLS}} / P_{\text{TLS}}$  with Formula (B.3).

$$\frac{dP_{\text{TLS},j}}{P_{\text{TLS},j}} = \sum_{i=1}^m \frac{|P_{\text{meas}+1,i} - P_{\text{meas},i}|}{m} / \sum_{i=1}^m \frac{P_{\text{meas},i}}{m} \quad (\text{B.3})$$

- g) Repeat the measurements for a few ( $j$ ) optical powers covering the desired power range. Calculate the power setting resolutions with Formula (B.4).

$$\frac{dP_{\text{TLS}}}{P_{\text{TLS}}} = \max\left(\frac{dP_{\text{TLS},j}}{P_{\text{TLS},j}}\right) \quad (\text{B.4})$$


## B.4 Signal-to-source spontaneous emission ratio

### B.4.1 General

Clause B.4 describes how to determine the side-mode suppression ratio (SMSR) of a laser with SSSER that can be measured with an OSA (e.g. SSSER of 60 dB). However, in the case of narrow line width laser sources such as an external cavity laser, the purity of the source can be much higher (around 90 dB) and therefore other methods can be used.

### B.4.2 Set-up

Figure B.3 shows the test set-up for a signal-to-source spontaneous emission ratio under standard test conditions.

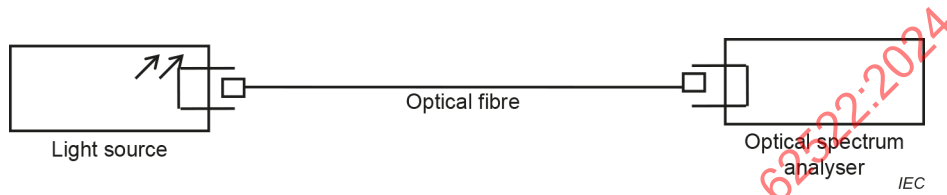

**Figure B.3 – Measurement set-up for signal to total source spontaneous emission ratio**

### B.4.3 Testing equipment

The OSA is used to measure the optical signal power and the spontaneous emission light.

### B.4.4 Testing procedure for determining signal-to-source spontaneous emission ratio

The testing procedure is as follows:

- Set the wavelength of the test light source to  $\lambda_{\text{TLS}}$ . Set the optical output power to a suitable value. Usually, the optical power is set to the maximum optical output power defined by the specifications of the test light source.
- Set the wavelength, the wavelength sweep range, and the resolution bandwidth of an OSA to  $\lambda_{\text{TLS}}$ ,  $\lambda_{\text{span}}$ , and  $\lambda_{\text{res}}$  respectively. Usually,  $\lambda_{\text{span}}$  is approximately 100 nm, and  $\lambda_{\text{res}}$  is approximately 1 nm.
- Inject the optical output of the light source into the OSA. Measure the optical signal optical power for  $P_1$ . Measure the maximum value  $P_2$  of a spontaneous emission optical level in  $\lambda_{\text{TLS}} \pm \Delta\lambda$ . However, the  $\lambda_{\text{TLS}} \pm \Delta\lambda_{\text{exc}}$  range will not be included as the measurement range of the spontaneous emission light (refer to Figure B.4). Usually,  $\Delta\lambda$  is approximately 50 nm,  $\Delta\lambda_{\text{exc}}$  is approximately 1 nm.
- Calculate the signal-to-source spontaneous emission ratio with Formula (B.5).


$$\text{SSER} = -10 \log \frac{P_2 \times 1 / \lambda_{\text{res}}}{P_1} \text{ dB/nm} \quad (\text{B.5})$$

where

SSER is the signal to source spontaneous emission ratio (dB/nm);

$P_1$  and  $P_2$  are in mW

$\lambda_{\text{res}}$  is in nm

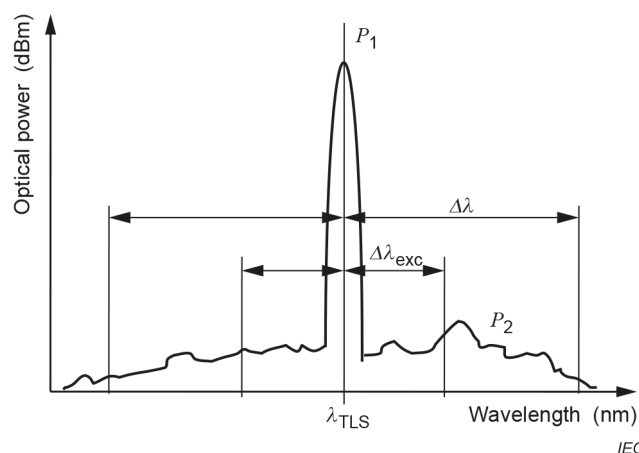

**Figure B.4 – Measurement of the signal to spontaneous emission ratio**

NOTE For a TLS with a high SSER, the optical rejection ratio of the OSA can limit the measured value.

Record the ratio of signal optical power and the spontaneous emission light as well as the measurement results.

## B.5 Side-mode suppression ratio


### B.5.1 General

In general, SMSR of a laser source can be measured with an OSA as described in IEC 61280-1-3:2021, 8.8. In the case of narrow line width laser sources such as an external cavity laser, however, the quite close interval between the main and side mode can cause difficulty to distinguish them with an OSA. Clause A.5 describes how to determine the SMSR of such a narrow line width laser source.

NOTE The testing approach adopted here measures the impact of SMSR on relative intensity noise (RIN), but possibly underestimates the power of the sidemodes when they are not in phase.

### B.5.2 Set-up

A special testing system is necessary, although it is performed by the tuneable laser source. For example, Figure B.5 shows the diagram of the test system of the SMSR test under standard test conditions.

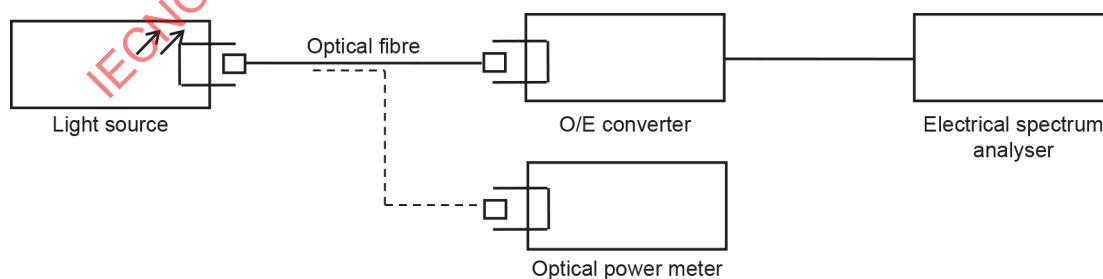

IEC

**Figure B.5 – Measurement set-up for the side-mode suppression ratio test**

### B.5.3 Testing equipment

Testing equipment is as follows:

- O/E (optical-electrical) converter: this is used for heterodyne detection of the intermode beat spectrum between the signal light and the side mode light, converting the optical signal to an electric signal. The frequency band should be several times wider than its mode spacing. The optical-electrical conversion efficiency should be calibrated beforehand.
- Electrical spectrum analyser: this is used to measure the beat signal level combined with the signal light and the side mode light.
- Optical power meter: this is used to measure the optical signal power.

### B.5.4 Testing procedure for determining the side-mode suppression ratio

The testing procedure is as follows:

- Set the wavelength of the light source to  $\lambda_{\text{TLS}}$ . Set the optical output power to a suitable value.
- Inject the optical output of the light source into to the O/E converter, and set the largest signal of the displayed beat signals measured by the spectrum analyser to  $P_{\text{beat,max}}$  (dBm).
- Next, inject the optical output of the light source into a optical power meter to measure the signal power. Set this value to  $P_0$  (dBm).
- Calculate the SMSR (dB) in wavelength  $\lambda_{\text{TLS}}$  with Formula (B.6).

$$\begin{aligned} \text{SMSR} &= 10\log \frac{P_0}{P_{\text{s,max}}} \\ &= 2P_0 - P_{\text{beat,max}} + R + 10\log(8R_i) - 30 \end{aligned} \quad (\text{B.6})$$

where

$P_{\text{s,max}}$  is a maximum side mode optical power (dBm);


$R$  is the conversion efficiency of O/E converter (dB);

$$R_{\text{dB}} = 20\log \frac{R}{1} \quad (\text{B.7})$$

$R_i$  is input impedance of OSA ( $\Omega$ ).

The following explains the measurement principle and Formula (B.6) for the SMSR.

It is assumed that the optical output spectrum of the test light source is composed with the side mode ( $P_s$ ) that is away from  $\Delta\Omega$  and the signal light ( $P_0$ ) – see Figure B.6.

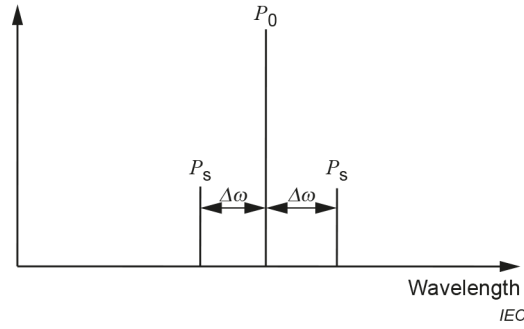

**Figure B.6 – Optical spectrum of tuneable laser source**

When the signal enters the measurement system shown in Figure B.7, the output current  $i_E$  of the O/E converter is calculated with Formula (B.8):

$$i_E = R \left\{ P_0 + 2P_s + 4\sqrt{P_0 P_s} \cos(\Delta\omega t) \right\} \quad (\text{B.8})$$

where

$R$  is a conversion efficiency of the O/E converter (A/W).


From Formula (B.8) when the beat current emerging from the signal light and the side mode is  $i_b$ , the beat signal power (electric)  $P_b$ , which is measured with the spectrum analyser, will be calculated with Formula (B.9) and Formula (B.10).

$$i_b = 4R\sqrt{P_0 P_s} \cos(\Delta\omega t) \quad (\text{B.9})$$

$$P_b = 8R_i P_0 P_s R^2 \quad (\text{B.10})$$

where

$R_i$  is the input impedance of the spectrum analyser ( $\Omega$ ).

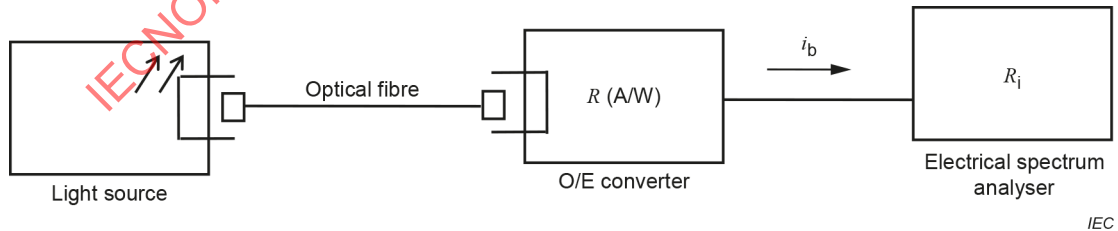

**Figure B.7 – Measurement set-up for SMSR**

The SMSR, derived from Formula (B.10), is calculated with Formula (B.11):

$$\text{SMSR} = \frac{P_0}{P_s} = 8R_i R^2 \frac{P_0^2}{P_b} \quad (\text{B.11})$$

If the SMSR is in dB, it will be calculated with Formula (B.12):

$$\begin{aligned} \text{SMSR}_{\text{dB}} &= 10\log\left(8R_i R^2 \frac{P_0^2}{P_b}\right) \\ &= 2P_{0,\text{dBm}} - P_{b,\text{dBm}} + R_{\text{dB}} + 10\log(8R_i) - 30 \end{aligned} \quad (\text{B.12})$$

where

$$P_{0,\text{dBm}} = 10\log \frac{P_0}{10^{-3}};$$

$$P_{b,\text{dBm}} = 10\log \frac{P_b}{10^{-3}};$$

$$R_{\text{dB}} = 20\log \frac{R}{1}.$$

NOTE The testing approach adopted here is suitable for external cavity lasers only.

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## Annex C (informative)

### Linear to dB scale conversion of uncertainties

#### C.1 Definition of decibel

The decibel is a submultiple of the bel (1 dB = 0,1 B). This unit is used to express values of power level on a logarithmic scale. The power level is always relative to a reference power  $P_0$ :

$$L_{P/P_0} = 10 \times \log_{10} \left( \frac{P}{P_0} \right) \text{ (dB)} \quad (\text{C.1})$$

where

$P$  and  $P_0$  are expressed in the same linear units.

#### C.2 Conversion of relative uncertainties

Similar to the previous definition, relative uncertainties,  $U_{\text{lin}}$ , or relative deviations, can be expressed in decibels:

$$U_{\text{dB}} = 10 \times \log_{10} (1 + U_{\%}) \quad (\text{C.2})$$

Reciprocally,  $U_{\text{lin}}$  can be expressed in % using:

$$U_{\%} = \left[ 10^{\left( \frac{U_{\text{dB}}}{10} \right)} - 1 \right] \times 100 \quad (\text{C.3})$$

For small values of  $U_{\text{lin}}$ , the first term of the applicable Taylor series can be used. Having:

$$\ln(1+x) = \sum_{n=1}^{\infty} \frac{-1^{n+1}}{n} x^n \text{ and } \log_{10}(x) = \frac{\ln(x)}{\ln(10)} \quad (\text{C.4})$$

that leads to:

$$U_{\text{dB}} = \frac{10}{\ln(10)} \sum_{n=1}^{\infty} \frac{-1^{n+1}}{n} U_{\text{lin}}^n \approx \frac{10}{\ln(10)} U_{\text{lin}} \quad (\text{C.5})$$

and two useful expressions:

$$U_{\text{dB}} \approx 4,34 \times U_{\text{lin}} \Leftrightarrow U_{\text{lin}} \approx 0,23 \times U_{\text{dB}} \quad (\text{C.6})$$

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## Bibliography

IEC 60027-3, *Letter symbols to be used in electrical technology – Part 3: Logarithmic and related quantities, and their units*

IEC 60050-300, *International Electrotechnical Vocabulary – Electrical and electronic measurements and measuring instruments – Part 311: General terms relating to measurements – Part 312: General terms relating to electrical measurements – Part 313: Types of electrical measuring instruments – Part 314: Specific terms according to the type of instrument*, available at [www.electropedia.org](http://www.electropedia.org)

IEC 60050-731, *International Electrotechnical Vocabulary – Chapter 731: Optical fibre communication*, available at [www.electropedia.org](http://www.electropedia.org)

IEC 60359, *Electrical and electronic measuring equipment – Expression of performance*

IEC 60793-1 (all parts), *Optical fibres – Part 1: Measurement methods and test procedures*

IEC 60793-2, *Optical fibres – Part 2: Product specifications – General*

IEC 61280-1-3:2021, *Fibre optic communication subsystem test procedures – Part 1-3: General communication subsystems – Measurement of central wavelength, spectral width and additional spectral characteristics*

IEC 61300-3-2, *Fibre optic interconnecting devices and passive components – Basic test and measurement procedures – Part 3-2: Examination and measurements – Polarization dependent loss in a single-mode fibre optic device*

IEC TR 61930, *Fibre optic graphical symbology*

IEC TR 61931, *Fibre optic – Terminology*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO/IEC Guide 99:2007, *International vocabulary of metrology – Basic and general concepts and associated terms (VIM)*

ISO 80000-3, *Quantities and units – Part 3: Space and time*

ITU-T G.694 (all parts), *Spectral grids for WDM applications*

ITU-T G. 694.1, *Spectral grids for WDM applications: DWDM frequency grid*

---

## SOMMAIRE

|                                                                                        |    |
|----------------------------------------------------------------------------------------|----|
| AVANT-PROPOS .....                                                                     | 43 |
| INTRODUCTION.....                                                                      | 45 |
| 1 Domaine d'application .....                                                          | 46 |
| 2 Références normatives .....                                                          | 46 |
| 3 Termes, définitions et abréviations .....                                            | 46 |
| 3.1 Termes et définitions .....                                                        | 46 |
| 3.2 Abréviations.....                                                                  | 49 |
| 4 Préparation pour l'étalonnage.....                                                   | 49 |
| 4.1 Organisation .....                                                                 | 49 |
| 4.2 Traçabilité.....                                                                   | 49 |
| 4.3 Préparation .....                                                                  | 50 |
| 4.4 Conditions d'étalonnage de référence .....                                         | 50 |
| 5 Étalonnage de la longueur d'onde .....                                               | 50 |
| 5.1 Présentation .....                                                                 | 50 |
| 5.2 Étalonnage de la longueur d'onde dans des conditions de référence.....             | 51 |
| 5.2.1 Montage .....                                                                    | 51 |
| 5.2.2 Équipement d'étalonnage .....                                                    | 51 |
| 5.2.3 Procédure d'étalonnage de la longueur d'onde .....                               | 51 |
| 5.2.4 Dépendance par rapport aux conditions.....                                       | 53 |
| 5.2.5 Incertitude dans les conditions de référence .....                               | 55 |
| 5.3 Étalonnage de la longueur d'onde dans les conditions de fonctionnement.....        | 56 |
| 5.3.1 Généralités.....                                                                 | 56 |
| 5.3.2 Dépendance par rapport à la puissance optique .....                              | 56 |
| 5.3.3 Incertitude aux conditions de fonctionnement .....                               | 57 |
| 6 Étalonnage de la puissance optique .....                                             | 57 |
| 6.1 Présentation .....                                                                 | 57 |
| 6.2 Étalonnage de la puissance optique dans les conditions de référence .....          | 58 |
| 6.2.1 Montage .....                                                                    | 58 |
| 6.2.2 Équipement d'étalonnage .....                                                    | 58 |
| 6.2.3 Procédure d'étalonnage de la puissance dans des conditions de<br>référence ..... | 59 |
| 6.2.4 Dépendance par rapport aux conditions.....                                       | 60 |
| 6.2.5 Incertitude dans les conditions de référence .....                               | 63 |
| 6.3 Étalonnage de la puissance optique dans les conditions de fonctionnement .....     | 64 |
| 6.3.1 Généralités.....                                                                 | 64 |
| 6.3.2 Dépendance par rapport à la longueur d'onde .....                                | 64 |
| 6.3.3 Incertitude aux conditions de fonctionnement .....                               | 65 |
| 7 Documentation .....                                                                  | 66 |
| 7.1 Données d'étalonnage et incertitude .....                                          | 66 |
| 7.2 Conditions d'étalonnage.....                                                       | 66 |
| Annexe A (normative) Base mathématique pour les calculs d'incertitude de mesure .....  | 67 |
| A.1 Généralités .....                                                                  | 67 |
| A.2 Évaluation de l'incertitude de type A .....                                        | 67 |
| A.3 Évaluation de l'incertitude de type B .....                                        | 68 |
| A.4 Détermination de l'incertitude-type combinée .....                                 | 69 |
| A.5 Rapport.....                                                                       | 69 |
| Annexe B (informative) Autres essais .....                                             | 70 |

|                        |                                                                                             |    |
|------------------------|---------------------------------------------------------------------------------------------|----|
| B.1                    | Généralités .....                                                                           | 70 |
| B.2                    | Résolution de l'accord de longueur d'onde .....                                             | 70 |
| B.2.1                  | Montage .....                                                                               | 70 |
| B.2.2                  | Équipement d'essai .....                                                                    | 70 |
| B.2.3                  | Procédure d'essai de détermination de la résolution de la longueur d'onde .....             | 70 |
| B.3                    | Résolution de l'accord de puissance optique .....                                           | 71 |
| B.3.1                  | Montage .....                                                                               | 71 |
| B.3.2                  | Équipement d'essai .....                                                                    | 71 |
| B.3.3                  | Procédure d'essai de la résolution de la puissance optique .....                            | 71 |
| B.4                    | Taux d'émission spontanée entre signal et source .....                                      | 72 |
| B.4.1                  | Généralités .....                                                                           | 72 |
| B.4.2                  | Montage .....                                                                               | 72 |
| B.4.3                  | Équipement d'essai .....                                                                    | 72 |
| B.4.4                  | Procédure d'essai pour déterminer le taux d'émission spontanée entre signal et source ..... | 73 |
| B.5                    | Taux de suppression des modes latéraux .....                                                | 74 |
| B.5.1                  | Généralités .....                                                                           | 74 |
| B.5.2                  | Montage .....                                                                               | 74 |
| B.5.3                  | Équipement d'essai .....                                                                    | 74 |
| B.5.4                  | Procédure d'essai pour déterminer le taux de suppression des modes latéraux .....           | 75 |
| Annexe C (informative) | Conversion linéaire en échelle dB des incertitudes .....                                    | 78 |
| C.1                    | Définition de décibels .....                                                                | 78 |
| C.2                    | Conversion des incertitudes relatives .....                                                 | 78 |
| Bibliographie .....    |                                                                                             | 79 |
| Figure 1               | – Montage de mesure de l'étalonnage de la longueur d'onde .....                             | 51 |
| Figure 2               | – Montage de mesure de la dépendance par rapport à la température .....                     | 53 |
| Figure 3               | – Montage de mesure de la stabilité de la longueur d'onde .....                             | 54 |
| Figure 4               | – Montage de mesure de la dépendance par rapport à la puissance optique .....               | 56 |
| Figure 5               | – Montage de mesure de l'étalonnage de la puissance optique intrinsèque .....               | 58 |
| Figure 6               | – Montage de mesure de la dépendance par rapport à la température .....                     | 60 |
| Figure 7               | – Montage de mesure de la stabilité de la puissance optique .....                           | 61 |
| Figure 8               | – Montage de mesure de la répétabilité/reproductibilité des connexions .....                | 62 |
| Figure 9               | – Montage de mesure de la dépendance à la longueur d'onde .....                             | 64 |
| Figure B.1             | – Montage de mesure de la résolution de la longueur d'onde .....                            | 70 |
| Figure B.2             | – Montage de mesure pour l'essai de réglage de résolution de la puissance optique .....     | 71 |
| Figure B.3             | Figure B.3 — Montage de mesure du taux d'émission spontanée entre signal et source .....    | 72 |
| Figure B.4             | – Mesure du taux d'émission spontanée entre signal et source .....                          | 73 |
| Figure B.5             | – Montage de mesure pour l'essai du taux de suppression des modes latéraux .....            | 74 |
| Figure B.6             | – Spectre optique de la source laser accordable .....                                       | 75 |
| Figure B.7             | – Montage de mesure pour le SMSR .....                                                      | 76 |
| Tableau 1              | – Source d'incertitude pour l'étalonnage de la longueur d'onde .....                        | 51 |

|                                                                                  |    |
|----------------------------------------------------------------------------------|----|
| Tableau 2 – Source d’incertitude pour l’étalonnage de la puissance optique ..... | 58 |
|----------------------------------------------------------------------------------|----|

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## COMMISSION ÉLECTROTECHNIQUE INTERNATIONALE

## ÉTALONNAGE DES SOURCES LASER ACCORDABLES

## AVANT-PROPOS

- 1) La Commission Électrotechnique Internationale (IEC) est une organisation mondiale de normalisation composée de l'ensemble des comités électrotechniques nationaux (Comités nationaux de l'IEC). L'IEC a pour objet de favoriser la coopération internationale pour toutes les questions de normalisation dans les domaines de l'électricité et de l'électronique. À cet effet, l'IEC – entre autres activités – publie des Normes internationales, des Spécifications techniques, des Rapports techniques, des Spécifications accessibles au public (PAS) et des Guides (ci-après dénommés "Publication(s) de l'IEC"). Leur élaboration est confiée à des comités d'études, aux travaux desquels tout Comité national intéressé par le sujet traité peut participer. Les organisations internationales, gouvernementales et non gouvernementales, en liaison avec l'IEC, participent également aux travaux. L'IEC collabore étroitement avec l'Organisation Internationale de Normalisation (ISO), selon des conditions fixées par accord entre les deux organisations.
- 2) Les décisions ou accords officiels de l'IEC concernant les questions techniques représentent, dans la mesure du possible, un accord international sur les sujets étudiés, étant donné que les Comités nationaux de l'IEC intéressés sont représentés dans chaque comité d'études.
- 3) Les Publications de l'IEC se présentent sous la forme de recommandations internationales et sont agréées comme telles par les Comités nationaux de l'IEC. Tous les efforts raisonnables sont entrepris afin que l'IEC s'assure de l'exactitude du contenu technique de ses publications; l'IEC ne peut pas être tenue responsable de l'éventuelle mauvaise utilisation ou interprétation qui en est faite par un quelconque utilisateur final.
- 4) Dans le but d'encourager l'uniformité internationale, les Comités nationaux de l'IEC s'engagent, dans toute la mesure possible, à appliquer de façon transparente les Publications de l'IEC dans leurs publications nationales et régionales. Toutes divergences entre toutes Publications de l'IEC et toutes publications nationales ou régionales correspondantes doivent être indiquées en termes clairs dans ces dernières.
- 5) L'IEC elle-même ne fournit aucune attestation de conformité. Des organismes de certification indépendants fournissent des services d'évaluation de conformité et, dans certains secteurs, accèdent aux marques de conformité de l'IEC. L'IEC n'est responsable d'aucun des services effectués par les organismes de certification indépendants.
- 6) Tous les utilisateurs doivent s'assurer qu'ils sont en possession de la dernière édition de cette publication.
- 7) Aucune responsabilité ne doit être imputée à l'IEC, à ses administrateurs, employés, auxiliaires ou mandataires, y compris ses experts particuliers et les membres de ses comités d'études et des Comités nationaux de l'IEC, pour tout préjudice causé en cas de dommages corporels et matériels, ou de tout autre dommage de quelque nature que ce soit, directe ou indirecte, ou pour supporter les coûts (y compris les frais de justice) et les dépenses découlant de la publication ou de l'utilisation de cette Publication de l'IEC ou de toute autre Publication de l'IEC, ou au crédit qui lui est accordé.
- 8) L'attention est attirée sur les références normatives citées dans cette publication. L'utilisation de publications référencées est obligatoire pour une application correcte de la présente publication.
- 9) L'IEC attire l'attention sur le fait que la mise en application du présent document peut entraîner l'utilisation d'un ou de plusieurs brevets. L'IEC ne prend pas position quant à la preuve, à la validité et à l'applicabilité de tout droit de propriété revendiqué à cet égard. À la date de publication du présent document, l'IEC avait/n'avait pas reçu notification qu'un ou plusieurs brevets pouvaient être nécessaires à sa mise en application. Toutefois, il y a lieu d'avertir les responsables de la mise en application du présent document que des informations plus récentes sont susceptibles de figurer dans la base de données de brevets, disponible à l'adresse <https://patents.iec.ch>. L'IEC ne saurait être tenue pour responsable de ne pas avoir identifié de tels droits de brevet.

L'IEC 62522 a été établie par le comité d'études 86 de l'IEC: Fibres optiques. Il s'agit d'une Norme internationale.

Cette deuxième édition annule et remplace la première édition parue en 2014. Cette édition constitue une révision technique.

Cette édition inclut les modifications techniques majeures suivantes par rapport à l'édition précédente:

- a) ajout de références à l'IEC 61315;
- b) ajout du Tableau 1 et du Tableau 2 sur les incertitudes;
- c) clarification des paramètres du wattmètre de référence en 6.2.3 et 6.3.2.3.

Le texte de cette Norme internationale est issu des documents suivants:

| Projet      | Rapport de vote |
|-------------|-----------------|
| 86/639/FDIS | 86/643/RVD      |

Le rapport de vote indiqué dans le tableau ci-dessus donne toute information sur le vote ayant abouti à son approbation.

La langue employée pour l'élaboration de cette Norme internationale est l'anglais.

Le présent document a été rédigé selon les Directives ISO/IEC, Partie 2, il a été développé selon les Directives ISO/IEC, Partie 1 et les Directives ISO/IEC, Supplément IEC, disponibles sous [www.iec.ch/members\\_experts/refdocs](http://www.iec.ch/members_experts/refdocs). Les principaux types de documents développés par l'IEC sont décrits plus en détail sous [www.iec.ch/publications](http://www.iec.ch/publications).

Le comité a décidé que le contenu de ce document ne sera pas modifié avant la date de stabilité indiquée sur le site Web de l'IEC sous [webstore.iec.ch](http://webstore.iec.ch) dans les données relatives au document recherché. À cette date, le document sera

- reconduit,
- supprimé, ou
- révisé.

IECNORM.COM : Click to view the full PDF of IEC 62522:2024

## INTRODUCTION

Les systèmes de transmission par multiplexage par répartition en longueur d'onde (MRL) sont déployés dans les lignes optiques principales. Les recommandations UIT-T de la série G.694 décrivent des grilles de fréquences et de longueurs d'onde pour des applications MRL. Par exemple, la grille de fréquence de la recommandation UIT-T G.694.1 prend en charge un certain nombre d'espacements entre les canaux sur une plage allant de 12,5 GHz à 100 GHz et sur une plage plus large dispositifs MRL, tels qu'un réseau de guide d'onde (AWG, Arrayed Waveguide Grating), des multiplexeurs (MUX) et des démultiplexeurs (DMUX) basés sur un filtre à couche mince ou sur des réseaux, avec un espacement étroit entre les canaux, sont intégrés dans les systèmes de transmission MRL. Lors de la mesure des caractéristiques de tels dispositifs, des sources laser accordables en longueur d'onde sont utilisées la plupart du temps et sont nécessaires pour obtenir des performances bien étalonnées. L'incertitude sur les longueurs d'onde, la répétabilité du caractère accordable des longueurs d'onde, la stabilité de la longueur d'onde et la stabilité de la puissance optique de sortie sont des paramètres importants.

Une source laser accordable (TLS, Tuneable Laser Source) présente généralement les fonctionnalités suivantes:

- a) la longueur d'onde de sortie est accordable de manière continue dans une plage de longueurs d'onde comprise entre 1 260 nm ou plus et 1 675 nm ou moins (il convient que la sortie n'excite que le mode fondamental LP01 de la fibre);
- b) un port de sortie pour connecteurs de fibres optiques.

L'enveloppe du spectre représente un mode longitudinal unique avec une largeur à mi-hauteur (FWHM, Full-Width at Half-Maximum) de 0,1 nm au plus. Tout mode adjacent est inférieur d'au moins 20 dB par rapport au mode spectral principal (par exemple, une diode laser à rétroaction répartie [DFB-LD, Distributed Feedback Laser Diode], un laser à cavité externe, etc.).

# ÉTALONNAGE DES SOURCES LASER ACCORDABLES

## 1 Domaine d'application

Le présent document fournit une procédure fiable et reproductible pour étalonner la longueur d'onde et la puissance de sortie d'un laser accordable en fonction des instruments de référence tels que des wattmètres optiques et des appareils de mesure de longueur d'onde optique (y compris des fréquencesmètres optiques) dont la traçabilité a été préalablement étalonnée.

## 2 Références normatives

Les documents suivants sont cités dans le texte de sorte qu'ils constituent, pour tout ou partie de leur contenu, des exigences du présent document. Pour les références datées, seule l'édition citée s'applique. Pour les références non datées, la dernière édition du document de référence s'applique (y compris les éventuels amendements).

IEC 60793-2-50, *Fibres optiques — Partie 2-50: Spécifications de produits — Spécification intermédiaire pour les fibres unimodales de classe B*

IEC 60825-1, *Sécurité des appareils à laser — Partie 1: Classification des matériels et exigences*

IEC 60825-2, *Sécurité des appareils à laser — Partie 2: Sécurité des systèmes de télécommunication par fibres optiques (STFO)*

IEC 61315, *Étalonnage de wattmètres pour dispositifs à fibres optiques*

IEC 62129-2, *Étalonnage des appareils de mesure de longueur d'onde/appareil de mesure de la fréquence optique — Partie 2: Appareils de mesure de longueur d'onde unique à interféromètre de Michelson*

ISO/IEC Guide 98-3:2008, *Incertitude de mesure — Partie 3: Guide pour l'expression de l'incertitude de mesure (GUM:1995)*

## 3 Termes, définitions et abréviations

### 3.1 Termes et définitions

Pour les besoins du présent document, les termes et définitions suivants s'appliquent.

L'ISO et l'IEC tiennent à jour des bases de données terminologiques destinées à être utilisées en normalisation, consultables aux adresses suivantes:

- IEC Electropedia: disponible à l'adresse <https://www.electropedia.org/>
- ISO Online browsing platform: disponible à l'adresse <https://www.iso.org/obp>

#### 3.1.1

##### **laboratoire d'étalonnage accrédité**

laboratoire d'étalonnage autorisé par l'organisation nationale compétente à publier des certificats d'étalonnage qui démontrent la traçabilité aux étalons nationaux

### 3.1.2

#### **ajustage**

ensemble des opérations réalisées sur un appareil pour qu'il fournisse des indications données correspondant à des valeurs données du mesurande

Note 1 à l'article: Pour plus d'informations, voir l'ISO/IEC Guide 99:2007, 3.11.

[SOURCE: IEC 60050-311:2001, 311-03-16, modifié — Le domaine a été supprimé, le terme "appareil de mesure" a été supprimé de la définition et la Note à l'article correspondante a été omise.]

### 3.1.3

#### **étalonnage**

ensemble des opérations qui, dans des conditions spécifiées, établissent une relation entre les valeurs des grandeurs indiquées par un appareil de mesure et les valeurs correspondantes fournies par des étalons

Note 1 à l'article: Le résultat d'un étalonnage permet soit l'affectation des valeurs d'un mesurande aux indications, soit la détermination de corrections par rapport aux indications.

Note 2 à l'article: Un étalonnage peut également déterminer d'autres propriétés métrologiques, telles que l'effet des grandeurs d'influence.

Note 3 à l'article: Le résultat d'un étalonnage peut être enregistré dans un document, appelé certificat d'étalonnage ou rapport d'étalonnage.

Note 4 à l'article: Voir également l'ISO/IEC Guide 99:2007, 2.39.

### 3.1.4

#### **conditions d'étalonnage**

conditions de mesure dans lesquelles l'étalonnage est réalisé

### 3.1.5

#### **étalonnage dans les conditions de référence**

étalonnage qui inclut l'évaluation de l'incertitude dans les conditions de référence de la source de rayonnement lumineux à étalonner

### 3.1.6

#### **étalonnage dans les conditions de fonctionnement**

étalonnage qui inclut l'évaluation de l'incertitude dans les conditions de fonctionnement de la source de rayonnement lumineux à étalonner

### 3.1.7

#### **niveau de confiance**

estimation de la probabilité que la valeur réelle d'un paramètre mesuré se trouve dans la plage donnée

### 3.1.8

#### **facteur d'élargissement**

$k$

facteur utilisé pour calculer l'incertitude élargie  $U$  à partir de l'incertitude-type  $u$

### 3.1.9

#### écart de puissance optique

$D_P$

différence entre la puissance définie de la source de rayonnement lumineux à étalonner,  $P_{\text{TLS}}$ , et la puissance de référence correspondante,  $P_{\text{meas}}$ , mesurée par le wattmètre de référence

$$D_P = \frac{P_{\text{TLS}} - P_{\text{meas}}}{P_{\text{meas}}}$$

Note 1 à l'article: La puissance  $P$  est exprimée en unités linéaires, par exemple W.

Note 2 à l'article: L'écart est relatif, il n'a pas d'unité (il peut être exprimé en %).

### 3.1.10

#### conditions de fonctionnement

ensemble approprié de plages spécifiées de valeurs des grandeurs d'influence, généralement supérieures aux conditions de référence pour lesquelles les incertitudes d'un appareil de mesure sont spécifiées

Note 1 à l'article: Les conditions de fonctionnement et l'incertitude dans les conditions de fonctionnement sont généralement spécifiées par le fabricant à l'intention de l'utilisateur.

### 3.1.11

#### conditions de référence

conditions utilisées pour les essais de performance d'un appareil de mesure ou pour la comparaison entre les résultats des mesures

Note 1 à l'article: Les conditions de référence comprennent généralement les valeurs de référence ou les plages de référence pour les grandeurs d'influence affectant l'appareil de mesure.

### 3.1.12

#### taux de suppression des modes latéraux

SMSR

rapport de la puissance de crête entre le spectre du mode principal et le spectre du mode latéral le plus large, ceci dans une diode laser unimodale telle qu'une diode laser DFB-LD

Note 1 à l'article: Le taux de suppression des modes latéraux est généralement exprimé en dB.

### 3.1.13

#### longueur d'onde

longueur d'onde (dans le vide) d'une source de rayonnement lumineux

### 3.1.14

#### écart en longueur d'onde

$D_\lambda$

différence entre la longueur d'onde cible, définie sur la source de rayonnement lumineux à étalonner,  $\lambda_{\text{TLS}}$ , et la longueur d'onde mesurée,  $\lambda_{\text{meas}}$ , en nm ou en  $\mu\text{m}$

$$D_\lambda = \lambda_{\text{TLS}} - \lambda_{\text{meas}}$$

### 3.2 Abréviations

|        |                                                                       |
|--------|-----------------------------------------------------------------------|
| APC    | angled physical contact (contact physique à angles)                   |
| AWG    | arrayed waveguide grating (réseau sélectif planaire)                  |
| DFB-LD | distributed feedback laser diode (diode laser à rétroaction répartie) |
| DMUX   | démultiplexeurs                                                       |
| FWHM   | full-width at half-maximum (largeur à mi-hauteur)                     |
| MUX    | multiplexeurs                                                         |
| O/E    | optique-électrique                                                    |
| OSA    | optical spectrum analyser (analyseur de spectre optique)              |
| RIN    | relative intensity noise (intensité relative de bruit)                |
| SMSR   | side-mode suppression ratio (taux de suppression des modes latéraux)  |
| TLS    | tuneable laser source (source laser accordable)                       |
| MRL    | multiplexage par répartition en longueur d'onde                       |

## 4 Préparation pour l'étalonnage

### 4.1 Organisation

Il convient que le laboratoire d'étalonnage s'assure que des exigences d'étalonnage appropriées sont respectées.

NOTE Des recommandations relatives aux bonnes pratiques d'étalonnage peuvent être consultées dans l'ISO/IEC 17025.

Il convient qu'une procédure de mesure documentée soit établie pour chaque type d'étalonnage effectué, donnant des instructions de fonctionnement étape par étape et l'appareillage à utiliser.

### 4.2 Traçabilité

Il convient que le laboratoire d'étalonnage s'assure que des exigences appropriées sont respectées.

NOTE Des recommandations relatives aux bonnes pratiques d'étalonnage peuvent être consultées dans l'ISO/IEC 17025.

Tous les étalons utilisés dans le processus d'étalonnage doivent être étalonnés conformément à un programme documenté avec une traçabilité reconnue par les laboratoires d'étalons nationaux ou par les laboratoires d'étalonnage accrédités.

Il est conseillé de conserver plus d'un étalon à chaque niveau de la hiérarchie, de telle sorte que les performances de l'étalon puissent être vérifiées par comparaison au même niveau. S'assurer que tout autre appareil d'étalonnage ayant une influence significative sur les résultats d'étalonnage est étalonné.

### 4.3 Préparation

Les conditions d'environnement doivent être compatibles avec le niveau d'incertitude exigé pour l'étalonnage:

- a) les étalonnages doivent être réalisés dans un environnement propre;
- b) le contrôle et la commande de la température sont exigés;
- c) toutes les sources laser doivent fonctionner en toute sécurité (conformément à l'IEC 60825-1 et à l'IEC 60825-2);
- d) il convient d'examiner la sortie de la TLS avec un analyseur de spectre optique (OSA, Optical Spectrum Analyser) ayant une résolution suffisante pour résoudre la structure en mode longitudinal dans le but de vérifier le fonctionnement en unimodal.

La température recommandée est de 23 °C, par exemple (23 ± 2) °C. Laisser aux appareils d'étalonnage suffisamment de temps avant l'essai (un temps de 2 h est recommandé) pour atteindre l'équilibre dans leur environnement. Faire subir à la TLS un temps de mise en température conforme aux instructions du fabricant.

### 4.4 Conditions d'étalonnage de référence

Les conditions d'étalonnage de référence incluent généralement les paramètres suivants et, si nécessaire, leurs bandes de tolérance: date, température, humidité relative, pression atmosphérique, puissance optique affichée, longueur d'onde affichée, fibre, combinaison connecteur-raccord, largeur de bande (spectrale) et largeur de bande de résolution (résolution spectrale) définies. Sauf spécification contraire, utiliser une fibre amorce pour fibre optique unimodale de catégorie B1.1 ou B1.3 comme spécifié dans l'IEC 60793-2-50, ayant une longueur d'au moins 2 m. Il est souhaitable d'effectuer tout l'étalonnage dans une situation où les rétroreflexions sont négligeables. Ainsi, il convient d'utiliser des isolateurs et des connecteurs à angles chaque fois que la situation le permet.

Utiliser la TLS conformément aux spécifications et aux modes opératoires du fabricant. Lorsque cela est possible, sélectionner un ensemble de conditions et de paramètres d'étalonnage de manière à simuler les conditions de fonctionnement réelles de la TLS à étalonner. Sélectionner ces paramètres afin d'optimiser la précision de la TLS, comme indiqué dans les modes opératoires du fabricant.

Documenter les conditions comme spécifié à l'Article 7.

NOTE Les résultats d'étalonnage ne sont valables que pour l'ensemble des conditions d'étalonnage utilisées dans le processus d'étalonnage.

## 5 Étalonnage de la longueur d'onde

### 5.1 Présentation

Les facteurs à l'origine de l'incertitude sur la longueur d'onde de la source de rayonnement lumineux à étalonner sont les suivants:

- a) l'incertitude intrinsèque de la source de rayonnement lumineux à étalonner dans les conditions de référence, qui inclut les dépendances à la température et à la durée pour ces conditions strictes;
- b) les incertitudes dues aux dépendances à la puissance optique, la température et la durée telles que dans les étalonnages dans des conditions de fonctionnement élargies.

La liste de la source d'incertitude est résumée dans le Tableau 1.

**Tableau 1 – Source d’incertitude pour l’étalonnage de la longueur d’onde**


| Source d’incertitude                                     | Type d’origine                                        | Symbole                       |
|----------------------------------------------------------|-------------------------------------------------------|-------------------------------|
| Répétabilité                                             | Mesure                                                | $s_{\lambda_j}$               |
| Température                                              | Environnement                                         | $u_{\lambda_j, \Delta\Theta}$ |
| Stabilité                                                | Source de rayonnement lumineux à étalonner            | $u_{\lambda_j, \Delta t}$     |
| Résolution de longueur d’onde                            | Appareil de mesure de la longueur d’onde de référence | $u_{\lambda_j, \text{res}}$   |
| Étalonnage de l’appareil de mesure de la longueur d’onde | Appareil de mesure de la longueur d’onde de référence | $u_{\text{WM}, \lambda_j}$    |
| Puissance optique                                        | Source de rayonnement lumineux à étalonner            | $u_{\lambda_j, P}$            |

L’étalonnage de la longueur d’onde dans les conditions de référence, pour des longueurs d’onde discrètes, décrit en 5.2, est obligatoire. L’étalonnage dans les conditions de fonctionnement, décrit en 5.3, est facultatif.

**5.2 Étalonnage de la longueur d’onde dans des conditions de référence**

**5.2.1 Montage**

La Figure 1 représente un système d’étalonnage de la longueur d’onde. L’étalonnage est réalisé dans les conditions de référence données.

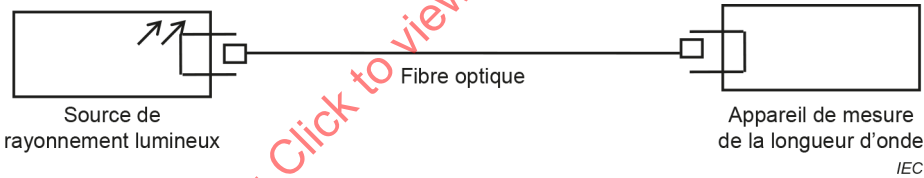

**Figure 1 – Montage de mesure de l’étalonnage de la longueur d’onde**

**5.2.2 Équipement d’étalonnage**

Un appareil de mesure de la longueur d’onde doit être utilisé pour l’étalonnage. L’appareil de mesure de la longueur d’onde doit être étalonné selon l’IEC 62129-2.

**5.2.3 Procédure d’étalonnage de la longueur d’onde**

La procédure d’étalonnage est la suivante:

- a) en utilisant le système d’étalonnage représenté sur la Figure 1, la longueur d’onde définie de la source de rayonnement lumineux est donnée par  $\lambda_{\text{TLS } j}$ , et les valeurs mesurées sont données par  $\lambda_{\text{meas } i, j}$ . L’incertitude de la mesure de la longueur d’onde tient compte de la répétabilité de l’ajustage et de l’hystérésis de la TLS. L’hystérésis est définie comme l’écart résultant de l’ajustage de la longueur d’onde souhaitée à partir à la fois de la longueur d’onde plus petite et de la longueur d’onde plus grande;
- b) il est recommandé de répéter la mesure de la longueur d’onde dix ( $(m)$ ) fois. S’assurer que la TLS est accordée sur  $\lambda_{\text{TLS } j}$  avant chaque mesure. Il convient que la longueur d’onde cible ( $j$ ) soit approchée d’une manière telle que l’accord se fait à la fois depuis la longueur d’onde plus petite et depuis la longueur d’onde plus grande;

- c) calculer la longueur d'onde mesurée moyenne  $\bar{\lambda}_{\text{meas } j}$  :

$$\bar{\lambda}_{\text{meas } j} = \frac{1}{m} \sum_{i=1}^m \lambda_{\text{meas } i, j} \quad (1)$$

où

$m$  est le nombre de mesures réalisées

il est pris pour hypothèse que chaque  $\lambda_{\text{meas } i, j}$  est une valeur moyenne de l'appareil de mesure de la longueur d'onde;

- d) calculer l'écart en longueur d'onde  $D_{\lambda_j}$  :

$$D_{\lambda_j} = \lambda_{\text{TLS } j} - \bar{\lambda}_{\text{meas } j} \quad (2)$$

où  $\lambda_{\text{TLS } j}$  est la longueur d'onde accordée de la TLS;

- e) calculer l'écart-type pour  $\lambda_j$  à partir des ( $m$ ) résultats de mesure de la longueur d'onde  $\lambda_{\text{meas } i, j}$  :

$$s_{\lambda_j} = \left[ \frac{1}{m-1} \sum_{i=1}^m (\lambda_{\text{meas } i, j} - \bar{\lambda}_{\text{meas } j})^2 \right]^{\frac{1}{2}} \quad (3)$$

- f) calculer la répétabilité de l'accord de la longueur d'onde  $S_{\text{rep}, \lambda_j}$  :

$$S_{\text{rep}, \lambda_j} = 2 \times s_{\lambda_j} \quad (4)$$

NOTE Un niveau de confiance par défaut de 95 % est utilisé dans la Formule (4).


Cette procédure d'étalonnage doit être réalisée pour chaque longueur d'onde d'étalonnage. Un minimum de 10 longueurs d'onde discrètes, ou tous les 10 nm, y compris la première longueur d'onde, la longueur d'onde centrale et la dernière longueur d'onde de la plage doivent être mesurées.

## 5.2.4 Dépendance par rapport aux conditions

### 5.2.4.1 Dépendance par rapport à la température (facultative, si connue)

#### 5.2.4.1.1 Montage

La Figure 2 représente un système d'étalonnage concernant la dépendance par rapport à la température. Cet étalonnage est réalisé dans les conditions d'étalonnage de référence à l'exception de la température.

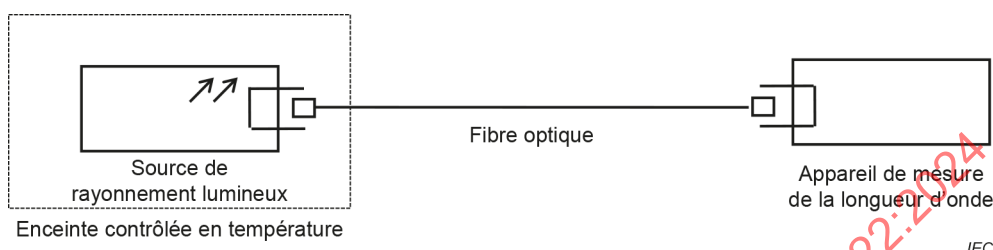

**Figure 2 – Montage de mesure de la dépendance par rapport à la température**

#### 5.2.4.1.2 Équipement d'étalonnage

L'équipement d'étalonnage est le suivant:

- un appareil de mesure de la longueur d'onde capable de détecter l'écart en longueur d'onde de la TLS en raison de la température;
- enceinte contrôlée en température: s'assurer que les résultats de mesure ne sont pas affectés par la répartition de la température interne.

#### 5.2.4.1.3 Procédure d'étalonnage concernant la détermination de la dépendance par rapport à la température

La procédure d'étalonnage est la suivante:

- en utilisant le système d'étalonnage de la Figure 2, mesurer la longueur d'onde nominale ( $j$ ) de la TLS à la puissance optique  $P_{\text{TLS}_j}$  dans les conditions de référence:  $\lambda_{j,\text{ref}}$ . Il convient que la longueur d'onde utilisée possède la réponse maximale aux variations de température. Sinon, il convient de caractériser plusieurs longueurs d'onde de sortie;
- mesurer la longueur d'onde de la TLS à la température ( $i$ ):  $\lambda_{j,\Theta_i}$ . Il convient de prendre la moyenne des longueurs d'onde lues correspondant à chaque réglage de température pour déterminer  $\lambda_{j,\Theta_i}$ ;
- calculer l'écart en longueur d'onde:

$$D_{\lambda_{j,\Theta_i}} = \lambda_{j,\Theta_i} - \lambda_{j,\text{ref}} \quad (5)$$

- d) répéter les étapes b) et c) avec  $(m)$  différents réglages de température  $\Theta_i$  en s'assurant que l'appareil dispose du temps nécessaire pour s'affranchir suffisamment de tout gradient thermique;
- e) calculer les écarts de longueur d'onde maximal  $\max\left(D_{\lambda_j, \Theta_i}\right)\Big|_{i=1}^{i=m}$  et minimal  $\min\left(D_{\lambda_j, \Theta_i}\right)\Big|_{i=1}^{i=m}$ ;
- f) l'incertitude-type concernant la dépendance de la longueur d'onde par rapport à la température  $u_{\lambda_j, \Delta\Theta}$ , à la longueur d'onde d'étalonnage  $(j)$ , en utilisant un modèle de distribution rectangulaire est:

$$u_{\lambda_j, \Delta\Theta} = \frac{1}{2\sqrt{3}} \left[ \max\left(D_{\lambda_j, \Theta_i}\right)\Big|_{i=1}^{i=m} - \min\left(D_{\lambda_j, \Theta_i}\right)\Big|_{i=1}^{i=m} \right] \quad (6)$$

où


$\Delta\Theta$  est la variation de température.

Il est recommandé de procéder à une acquisition de longueur d'onde avec l'appareil de mesure de la longueur d'onde optique pour la durée de cet étalonnage.

#### 5.2.4.2 Stabilité de la longueur d'onde

##### 5.2.4.2.1 Montage

La Figure 3 représente un système d'étalonnage de la stabilité de la longueur d'onde. Cet étalonnage est réalisé dans les conditions d'étalonnage de référence à l'exception du temps.

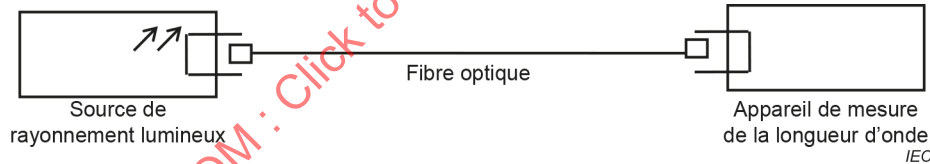

**Figure 3 – Montage de mesure de la stabilité de la longueur d'onde**

##### 5.2.4.2.2 Équipement d'étalonnage

Il est recommandé d'utiliser un appareil de mesure de la longueur d'onde capable de détecter les fluctuations de longueur d'onde de la TLS.

##### 5.2.4.2.3 Procédure d'étalonnage concernant la stabilité de la longueur d'onde

La procédure d'étalonnage est la suivante:

- a) une période  $(\Delta t)$  assez longue, par exemple 10 min, doit être choisie pour permettre de procéder à au moins 10 mesures de la longueur d'onde avec l'appareil de mesure de la longueur d'onde de référence (dans le cas de l'exemple, la stabilité est mesurée sur 10 min);
- b) il convient d'effectuer une acquisition continue de la longueur d'onde qui inclut les données de longueur d'onde et d'horodatage;
- c) s'assurer de corrélérer les  $(m)$  mesures par période, avec  $(m > 10)$  et exactement conforme à la période souhaitée  $(\Delta t)$ ;

- d) calculer l'écart-type pour les ( $m$ ) mesures de la longueur d'onde correspondant à la période ( $\Delta t$ );

$$u_{\lambda_j, \Delta t} = \left[ \frac{1}{m-1} \sum_{i=1}^m (\lambda_{j, t_i} - \frac{1}{m} \sum_{i=1}^m \lambda_{j, t_i})^2 \right]^{\frac{1}{2}} \quad (7)$$

- e) au minimum, 1 période est exigée pour évaluer la stabilité de la longueur d'onde de la TLS. Dans ce cas, l'incertitude sur la stabilité de la longueur d'onde devient:

$$S_{\text{stab}, \lambda_j, \Delta t} = 2 \times u_{\lambda_j, \Delta t} \quad (8)$$

NOTE Un niveau de confiance par défaut de 95 % est utilisé dans la Formule (8).

Il convient de mesurer la longueur d'onde de la source de rayonnement lumineux plus de dix fois ( $m$  fois) consécutivement. Il est recommandé d'effectuer au moins quelques mesures par minute. Il convient que l'intervalle de temps entre les mesures répétées soit plus long que le temps de réponse de la source de rayonnement lumineux. Il est préférable de calculer plusieurs périodes à partir des données d'acquisition en utilisant une fenêtre glissante et la valeur maximale est consignée.

### 5.2.5 Incertitude dans les conditions de référence

L'incertitude sur la longueur d'onde d'étalonnage ( $j$ ) dans les conditions de référence est donnée par:

$$u_{\lambda_j, \text{ref}} = \left( \frac{s_{\lambda_j}^2}{m} + u_{\lambda_j, \Delta \Theta}^2 + u_{\lambda_j, \Delta t}^2 + u_{\lambda_j, \text{res}}^2 + u_{\text{WM}_{\lambda_j}}^2 \right)^{\frac{1}{2}} \quad (9)$$

où

$u_{\lambda_j, \Delta \Theta}$  et  $u_{\lambda_j, \Delta t}$  sont évalués pour les conditions de référence telles qu'elles sont définies en 5.2.4;

$u_{\lambda_j, \text{res}}$  est l'incertitude sur la résolution de la longueur d'onde définie par

$$u_{\lambda_j, \text{res}} = d\lambda_j / 2\sqrt{3}$$

( $d\lambda_j$  est la résolution de longueur d'onde de l'appareil de mesure de la longueur d'onde);

$u_{\text{WM}_{\lambda_j}}$  est l'incertitude de l'appareil de mesure de la longueur d'onde à la longueur d'onde ( $j$ ) telle qu'elle est décrite dans sa certification;

l'incertitude élargie sur la longueur d'onde d'étalonnage ( $j$ ) dans les conditions de référence,  $U_{\lambda_j, \text{ref}}$ , avec un facteur d'élargissement  $k$  est exprimée comme suit:

$$U_{\lambda_j, \text{ref}} = k u_{\lambda_j, \text{ref}} \quad (10)$$

où

$k$  correspond à un niveau de confiance approprié comme cela est décrit à l'Article A.5.

Voir l'Annexe A et l'Annexe C pour plus d'informations sur les incertitudes.

Lorsque les réglages sont effectués sur l'appareil d'après les résultats d'étalonnage, il est recommandé de répéter les étalonnages après ces réglages pour vérifier les corrections.

### 5.3 Étalonnage de la longueur d'onde dans les conditions de fonctionnement

#### 5.3.1 Généralités

Effectuer la procédure d'étalonnage quand la source de rayonnement lumineux est utilisée au-delà des conditions de référence.


Les différents facteurs de l'incertitude sur la longueur d'onde dans les conditions de fonctionnement sont les suivants:

- a) dépendance par rapport à la puissance optique;
- b) dépendance par rapport à la température;
- c) stabilité de la longueur d'onde.

#### 5.3.2 Dépendance par rapport à la puissance optique

##### 5.3.2.1 Généralités

La Figure 4 représente un système d'étalonnage concernant la dépendance par rapport à la puissance optique. Il convient de procéder à cet étalonnage dans les conditions d'étalonnage de référence à l'exception de la puissance optique. Il doit être réalisé après l'étalonnage de la puissance optique (6.2.3).

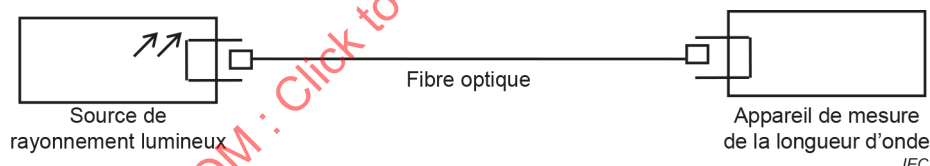

**Figure 4 – Montage de mesure de la dépendance par rapport à la puissance optique**

##### 5.3.2.2 Équipement d'étalonnage

L'appareil de mesure de la longueur d'onde doit être étalonné selon l'IEC 62129-2.

##### 5.3.2.3 Procédures d'étalonnage concernant la détermination de la dépendance par rapport à la puissance

Les procédures d'étalonnage sont les suivantes:

- a) la longueur d'onde ( $\lambda$ ) est mesurée à  $m$  puissances optiques de la source de rayonnement lumineux,  $P_{\text{TLS } i,j}$ , y compris les limites supérieures et inférieures de la plage de puissances spécifiée. Il convient que l'intervalle entre ces niveaux voisins soit inférieur à 10 dB;
- b) en utilisant le système d'étalonnage représenté sur la Figure 4, la longueur d'onde définie de la source de rayonnement lumineux est donnée par  $\lambda_{\text{TLS } i,j}$ , et les valeurs de l'appareil de mesure de la longueur d'onde sont données par  $\lambda_{P_{i,j}}$ ;

- c) enregistrer la longueur d'onde mesurée,  $\lambda_{P_{i,j}}$ , pour tous les ( $m$ ) réglages de la puissance de sortie  $P_{\text{TLS } i,j}$  utilisés;
- d) calculer l'incertitude-type sur la longueur d'onde ( $j$ ) due à la puissance optique de sortie de la TLS selon l'équation

$$u_{\lambda_j,P} = \left[ \frac{1}{m-1} \sum_{i=1}^m (\lambda_{P_{i,j}} - \frac{1}{m} \sum_{i=1}^m \lambda_{P_{i,j}})^2 \right]^{\frac{1}{2}} \quad (11)$$

### 5.3.3 Incertitude aux conditions de fonctionnement

L'incertitude sur la longueur d'onde d'étalonnage ( $j$ ) dans n'importe quelle condition de fonctionnement est donnée par

$$u_{\lambda_j,\text{op}} = \left( s_{\lambda_j}^2 + u_{\lambda_j,P}^2 + u_{\lambda_j,\Delta\Theta}^2 + u_{\lambda_j,\Delta t}^2 + u_{\lambda_j,\text{res}}^2 + u_{\text{WM}_{\lambda_j}}^2 \right)^{\frac{1}{2}} \quad (12)$$

où

$u_{\lambda_j,P}$ ,  $u_{\lambda_j,\Delta\Theta}$  et  $u_{\lambda_j,\Delta t}$  sont évalués pour les conditions de fonctionnement;

$u_{\lambda_j,\text{res}}$  est l'incertitude sur la résolution de longueur d'onde définie par  $u_{\lambda_j,\text{res}} = d\lambda_j / 2\sqrt{3}$  ( $d\lambda_j$  est la résolution de longueur d'onde de l'appareil de mesure de longueur d'onde);

$u_{\text{WM}_{\lambda_j}}$  est l'incertitude de l'appareil de mesure de la longueur d'onde à la longueur d'onde ( $j$ ) telle qu'elle est décrite dans sa certification;

l'incertitude élargie sur la longueur d'onde d'étalonnage ( $j$ ) dans toutes les conditions de fonctionnement,  $U_{\lambda_j,\text{op}}$  avec un facteur d'élargissement  $k$ , est exprimée comme suit:

$$U_{\lambda_j,\text{op}} = k u_{\lambda_j,\text{op}} \quad (13)$$

où

$k$  correspond à un niveau de confiance approprié comme cela est décrit à l'Article A.5.

## 6 Étalonnage de la puissance optique

### 6.1 Présentation

Les facteurs ayant une influence sur l'incertitude sur la puissance optique définie de la source de rayonnement lumineux à étalonner sont les suivants:

- a) l'incertitude intrinsèque de la source de rayonnement lumineux à étalonner dans des conditions de référence qui inclut les dépendances à la température, à la durée et à la répétabilité/reproductibilité des connexions pour ces conditions strictes;
- b) les incertitudes dues aux dépendances sur la longueur d'onde, la température, la durée et la répétabilité/reproductibilité des connexions, telles que dans les étalonnages aux conditions de fonctionnement élargies.

La liste de la source d'incertitude est résumée dans le Tableau 2.

**Tableau 2 – Source d'incertitude pour l'étalonnage de la puissance optique**


| Source d'incertitude               | Type d'origine                             | Symbole                 |
|------------------------------------|--------------------------------------------|-------------------------|
| Répétabilité                       | Mesure                                     | $s_{DP_j}$              |
| Température                        | Environnement                              | $u_{DP_j,\Delta\Theta}$ |
| Stabilité                          | Source de rayonnement lumineux à étalonner | $u_{DP_j,\Delta t}$     |
| Reproductibilité de connexion      | Source de rayonnement lumineux à étalonner | $u_{DP_j,con}$          |
| Résolution de la puissance optique | Wattmètre optique de référence             | $u_{DP_j,res}$          |
| Étalonnage du wattmètre optique    | Wattmètre optique de référence             | $u_{PM_{P_j}}$          |
| Longueur d'onde                    | Source de rayonnement lumineux à étalonner | $u_{DP_j,\lambda}$      |

L'étalonnage de la puissance optique dans des conditions de référence, comme décrit en 6.2, est obligatoire. L'étalonnage dans les conditions de fonctionnement, décrit en 6.3, est facultatif.

**6.2 Étalonnage de la puissance optique dans les conditions de référence**

**6.2.1 Montage**

La Figure 5 représente un système pour l'étalonnage de la puissance optique. L'étalonnage est réalisé dans les conditions de référence données.

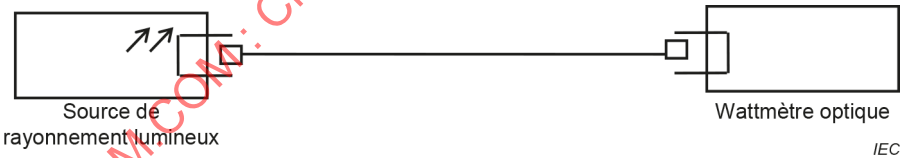

**Figure 5 – Montage de mesure de l'étalonnage de la puissance optique intrinsèque**

NOTE Des problèmes peuvent se produire lors de l'étalonnage de la puissance d'une source laser à cohérence élevée, en raison des effets des interférences parasites résultant des réflexions sur les faces d'extrémité des connecteurs de fibre et sur le wattmètre optique. L'utilisation de connecteurs à contact physique à angles (APC, Angled Physical Contact), d'isolateurs optiques intégrés et de la fonction de contrôle de cohérence des lasers (le cas échéant) peut réduire les effets des interférences à un niveau acceptable.

La puissance optique à étalonner est mesurée à l'extrémité d'un câble à fibre optique, ce qui peut provoquer des pertes d'insertion. Il convient de consigner les conditions d'étalonnage relatives au câble à fibre optique utilisé telles que la longueur de fibre, le type de connecteur, l'isolateur intégré (le cas échéant).

**6.2.2 Équipement d'étalonnage**

Le wattmètre optique doit être étalonné selon l'IEC 61315.

### 6.2.3 Procédure d'étalonnage de la puissance dans des conditions de référence

La procédure d'étalonnage est la suivante:

- raccorder la source de rayonnement lumineux et le wattmètre à la fibre optique;
- réglér la longueur d'onde de la source de rayonnement lumineux et du wattmètre optique à la longueur d'onde d'étalonnage exigée;
- réglér la puissance de sortie de la source de rayonnement lumineux sur  $P_{\text{TLS}j}$ . L'incertitude de la mesure de la puissance tient compte de la répétabilité du réglage et de l'hystérésis de la TLS. L'hystérésis est définie comme l'écart résultant du réglage de la puissance souhaitée à partir à la fois de la puissance inférieure et de la puissance supérieure;
- lire la valeur mesurée par le wattmètre optique;
- il est recommandé de répéter cette mesure dix ( $m$ ) fois. S'assurer que la TLS est réglée sur  $P_{\text{TLS}j}$  avant chaque mesure. Il convient que la puissance cible soit approchée d'une manière telle que le réglage se fait à la fois depuis la puissance inférieure et depuis la puissance supérieure;

$$D_{P_{i,j}} = \frac{P_{\text{TLS}j} - P_{\text{meas } i,j}}{P_{\text{meas } i,j}} \quad (14)$$

où

$P_{\text{TLS}j}$  est la puissance optique appliquée à la TLS

il est pris pour hypothèse que chaque  $P_{\text{meas } i,j}$  est une valeur moyenne du wattmètre. Calculer l'écart de puissance  $D_{P_j}$

$$D_{P_j} = \frac{1}{m} \sum_{i=1}^m D_{P_{i,j}} \quad (15)$$

où

$m$  est le nombre de mesures réalisées;

- calculer l'écart-type pour  $D_{P_j}$  à partir des ( $m$ ) résultats de mesure de la puissance  $P_{\text{meas } i,j}$ :

$$s_{D_{P_j}} = \left[ \frac{1}{m-1} \sum_{i=1}^m (D_{P_{i,j}} - D_{P_j})^2 \right]^{\frac{1}{2}} \quad (16)$$

- calculer la répétabilité du réglage de la puissance optique:  $S_{\text{rep}, D_{P_j}}$

$$S_{\text{rep}, D_{P_j}} = 2 \times s_{D_{P_j}} \quad (17)$$

NOTE Un niveau de confiance par défaut de 95 % est utilisé dans la Formule (17).


Il convient d'effectuer les calculs d'incertitude (6.2.3 a) à g)) pour chaque puissance d'étalonnage.

## 6.2.4 Dépendance par rapport aux conditions

### 6.2.4.1 Dépendance par rapport à la température (facultative, si connue)

#### 6.2.4.1.1 Montage

La Figure 6 représente un système d'étalonnage concernant la dépendance par rapport à la température. Cet étalonnage est réalisé dans les conditions d'étalonnage de référence à l'exception de la température.

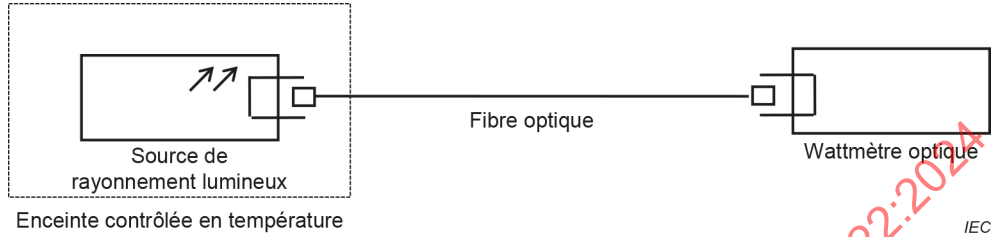

**Figure 6 – Montage de mesure de la dépendance par rapport à la température**

#### 6.2.4.1.2 Équipement d'étalonnage

L'équipement d'étalonnage est le suivant:

- un appareil de mesure optique capable de détecter l'écart de puissance optique de la TLS en fonction de la température;
- enceinte contrôlée en température:  
s'assurer que les résultats de mesure ne sont pas affectés par la répartition de la température interne.

#### 6.2.4.1.3 Procédure d'étalonnage concernant la détermination de la dépendance par rapport à la température

La procédure d'étalonnage est la suivante:

- en utilisant le système d'étalonnage de la Figure 6, mesurer la puissance optique nominale de la TLS à la longueur d'onde  $\lambda_{TLSj}$  dans les conditions de référence  $P_{j,ref}$ . Il convient que la puissance optique utilisée possède la réponse maximale par rapport aux variations de température; Sinon, il est nécessaire de caractériser plusieurs puissances optiques;
- mesurer la puissance optique de la TLS à la température ( $i$ ):  $P_{j,\Theta_i}$ . Il convient de prendre la moyenne des puissances optiques lues correspondant à chaque réglage de température pour déterminer  $P_{j,\Theta_i}$ ;
- calculer l'écart de puissance optique relative:

$$D_{P_{j,\Theta_i}} = \frac{P_{j,\Theta_i} - P_{j,ref}}{P_{j,ref}} \quad (18)$$

- répéter les étapes b) et c) avec ( $m$ ) différents réglages de température  $\Theta_i$  en s'assurant que l'appareil dispose du temps nécessaire pour s'affranchir suffisamment de tout gradient thermique;

- e) calculer les écarts de puissance optique maximal  $\max(D_{P_j, \Theta_i}) \Big|_{i=1}^{i=m}$  et minimal  $\min(D_{P_j, \Theta_i}) \Big|_{i=1}^{i=m}$  ;
- f) l'incertitude-type concernant la dépendance par rapport à la température de la puissance optique  $u_{P_j, \Delta\Theta}$  à la puissance optique d'étalonnage en utilisant un modèle de distribution rectangulaire est:

$$u_{D_{P_j, \Delta\Theta}} = \frac{1}{2\sqrt{3}} \left[ \max(D_{P_j, \Theta_i}) \Big|_{i=1}^{i=m} - \min(D_{P_j, \Theta_i}) \Big|_{i=1}^{i=m} \right] \quad (19)$$

où


$\Delta\Theta$  est la variation de température

il est recommandé de procéder à une acquisition de la puissance optique avec le wattmètre optique pour la durée de cet étalonnage.

## 6.2.4.2 Stabilité de la puissance optique

### 6.2.4.2.1 Montage

La Figure 7 représente un système d'étalonnage pour la stabilité de la puissance optique. Cet étalonnage est réalisé dans les conditions d'étalonnage de référence à l'exception du temps.

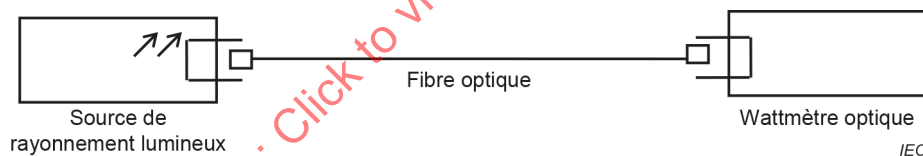

**Figure 7 – Montage de mesure de la stabilité de la puissance optique**

### 6.2.4.2.2 Équipement d'étalonnage

Il est recommandé d'utiliser un wattmètre optique capable de détecter les fluctuations de puissance optique de la TLS.

### 6.2.4.2.3 Procédure d'étalonnage concernant la stabilité de la puissance optique

La procédure d'étalonnage est la suivante:

- une période spécifique ( $\Delta t$ ) assez longue, par exemple 10 min, doit être choisie pour permettre de procéder à au moins 10 mesures de la puissance optique avec le wattmètre de référence (dans le cas de l'exemple, la stabilité est mesurée sur 10 min);
- il convient d'effectuer une acquisition continue de la puissance optique qui inclut les données de puissance optique et d'horodatage;
- s'assurer de corrélérer les ( $m$ ) mesures par période, avec ( $m > 10$ ) et exactement conforme à la période souhaitée ( $\Delta t$ );

d) calculer l'écart-type pour les ( $m$ ) mesures correspondant à la période ( $\Delta t$ ):

$$u_{D_{P_j, \Delta t}} = \left[ \frac{1}{m-1} \sum_{i=1}^m (P_{j, t_i} - \frac{1}{m} \sum_{i=1}^m P_{j, t_i})^2 \right]^{\frac{1}{2}} / \left( \frac{1}{m} \sum_{i=1}^m P_{j, t_i} \right) \quad (20)$$

e) au minimum, 1 période est exigée pour évaluer la stabilité de la puissance optique de la TLS. Dans ce cas, l'incertitude sur la stabilité de la puissance optique devient:

$$S_{\text{stab}, D_{P_j, \Delta t}} = 2 \times u_{D_{P_j, \Delta t}} \quad (21)$$

NOTE Un niveau de confiance par défaut de 95 % est utilisé dans la Formule (21).

Il est préférable de calculer plusieurs périodes à partir des données d'acquisition en utilisant une fenêtre glissante et la valeur maximale est consignée.

Il convient de mesurer la puissance optique de la source de rayonnement lumineux plus de dix fois ( $m$  fois) consécutivement. Il est recommandé d'effectuer au moins quelques mesures par minute. Il convient que l'intervalle de temps entre les mesures répétées soit plus long que le temps de réponse de la source de rayonnement lumineux.

### 6.2.4.3 Répétabilité/reproductibilité des connexions

#### 6.2.4.3.1 Montage

La Figure 8 représente un système d'étalonnage pour la stabilité de la puissance optique. Cet étalonnage est réalisé dans les conditions d'étalonnage de référence.

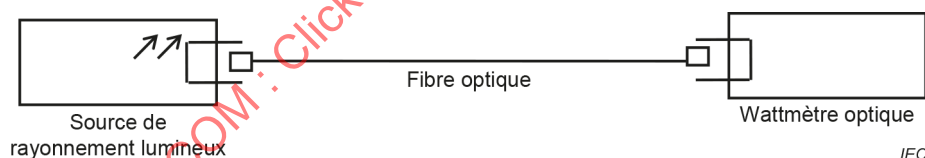


Figure 8 – Montage de mesure de la répétabilité/reproductibilité des connexions

#### 6.2.4.3.2 Équipement d'étalonnage

Le wattmètre optique doit être étalonné selon l'IEC 61315.

### 6.2.4.3.3 Procédure d'étalonnage concernant la répétabilité/reproductibilité des connexions

La procédure d'étalonnage est la suivante:

- en utilisant le système d'étalonnage de la Figure 8, raccorder la source de rayonnement lumineux et le wattmètre à la fibre optique;
- lire la valeur mesurée par le wattmètre optique  $P_{j,\text{con}_i}$ ;
- déconnecter la fibre optique de la TLS et reconnecter la fibre optique à la TLS;
- répéter les étapes b) et c) ( $m$ ) fois;
- calculer l'incertitude-type sur la puissance optique ( $j$ ) due à la répétabilité/reproductibilité des connexions selon l'équation

$$u_{D_{P_j,\text{con}}} = \left[ \frac{1}{m-1} \sum_{i=1}^m \left( P_{j,\text{con}_i} - \frac{1}{m} \sum_{i=1}^m P_{j,\text{con}_i} \right)^2 \right]^{\frac{1}{2}} / \left( \frac{1}{m} \sum_{i=1}^m P_{j,\text{con}_i} \right) \quad (22)$$

### 6.2.5 Incertitude dans les conditions de référence

L'incertitude sur la puissance optique d'étalonnage dans les conditions de référence est donnée par:

$$u_{D_{P_j,\text{ref}}} = \left( \frac{s_{D_{P_j}}^2}{m} + u_{D_{P_j,\Delta\Theta}}^2 + u_{D_{P_j,\Delta t}}^2 + u_{D_{P_j,\text{con}}}^2 + u_{D_{P_j,\text{res}}}^2 + u_{\text{PM}_{P_j}}^2 \right)^{\frac{1}{2}} \quad (23)$$

où

$u_{D_{P_j,\Delta\Theta}}$ ,  $u_{D_{P_j,\Delta t}}$  et  $u_{D_{P_j,\text{con}}}$  sont évalués pour les conditions de référence telles qu'elles sont définies en 6.2.4;

$u_{D_{P_j,\text{res}}}$  est l'incertitude relative sur la résolution de la puissance optique définie par  $u_{D_{P_j,\text{res}}} = (dP_{\text{TLS},j} / P_{\text{TLS},j}) / 2\sqrt{3}$  ( $dP_{\text{TLS},j}$  est la résolution de la puissance optique du wattmètre optique);

$u_{\text{PM}_{P_j}}$  est l'incertitude relative du wattmètre optique à la puissance  $P_j$  telle qu'elle est décrite dans sa certification.

L'incertitude élargie sur le wattmètre optique d'étalonnage aux conditions de référence  $U_{D_{P_j,\text{ref}}}$ , avec un facteur d'élargissement  $k$ , est exprimée comme suit:

$$U_{D_{P_j,\text{ref}}} = k u_{D_{P_j,\text{ref}}} \quad (24)$$

où

$k$  correspond à un niveau de confiance approprié comme cela est décrit à l'Article A.5.

Voir l'Annexe A pour plus d'informations sur les incertitudes.

Lorsque les réglages sont effectués sur l'appareil d'après les résultats d'étalonnage, il est recommandé de répéter les étalonnages après ces réglages pour vérifier les corrections.

## 6.3 Étalonnage de la puissance optique dans les conditions de fonctionnement

### 6.3.1 Généralités

Effectuer la procédure d'étalonnage quand la source de rayonnement lumineux est utilisée au-delà des conditions de référence.

Les différents facteurs de l'incertitude sur la puissance optique dans les conditions de fonctionnement sont les suivants:

- a) dépendance par rapport à la longueur d'onde;
- b) dépendance par rapport à la température;
- c) stabilité de la puissance optique;
- d) répétabilité/reproductibilité des connexions.

### 6.3.2 Dépendance par rapport à la longueur d'onde

#### 6.3.2.1 Montage

La Figure 9 représente un système d'étalonnage concernant la dépendance par rapport à la longueur d'onde. Il convient de réaliser cet étalonnage dans les conditions d'étalonnage de référence à l'exception de la longueur d'onde. Il doit être réalisé après l'étalonnage de la longueur d'onde (5.2.3).



**Figure 9 – Montage de mesure de la dépendance à la longueur d'onde**

#### 6.3.2.2 Équipement d'étalonnage

L'équipement d'étalonnage est le suivant: il convient d'étalonner le wattmètre optique selon l'IEC 61315.

#### 6.3.2.3 Procédure d'étalonnage concernant la détermination de la dépendance par rapport à la longueur d'onde

La procédure d'étalonnage est la suivante:

- a) la puissance optique est mesurée à  $m$  longueurs d'onde (plus de 5) de la source de rayonnement lumineux,  $\lambda_{\text{TLS } i,j}$  y compris les limites supérieures et inférieures de la plage de longueurs d'onde spécifiée;
- b) en utilisant le système d'étalonnage représenté sur la Figure 9, la puissance optique définie de la source de rayonnement lumineux est donnée par  $P_{\text{TLS } i,j}$ , et les valeurs du wattmètre sont données par  $P_{\lambda_i,j}$ ;
- c) régler la longueur d'onde du wattmètre optique à la longueur d'onde d'étalonnage exigée;

- d) enregistrer la puissance optique mesurée  $P_{\lambda_{i,j}}$  pour tous les ( $m$ ) réglages de la longueur d'onde  $\lambda_{\text{TLS } i,j}$  utilisés;
- e) calculer l'incertitude-type sur la puissance optique ( $j$ ) due à la longueur d'onde de sortie de la TLS selon:

$$u_{D_{P_j,\lambda}} = \left[ \frac{1}{m-1} \sum_{i=1}^m \left( P_{\lambda_{i,j}} - \frac{1}{m} \sum_{i=1}^m P_{\lambda_{i,j}} \right)^2 \right]^{\frac{1}{2}} / \left( \frac{1}{m} \sum_{i=1}^m P_{\lambda_{i,j}} \right) \quad (25)$$

### 6.3.3 Incertitude aux conditions de fonctionnement

L'incertitude sur la puissance optique d'étalonnage dans n'importe quelle condition de fonctionnement est donnée par:

$$u_{D_{P_j,op}} = \left( s_{D_{P_j}}^2 + u_{D_{P_j,\lambda}}^2 + u_{D_{P_j,\Delta\theta}}^2 + u_{D_{P_j,\Delta t}}^2 + u_{D_{P_j,con}}^2 + u_{D_{P_j,res}}^2 + u_{PM_{P_j}}^2 \right)^{\frac{1}{2}} \quad (26)$$

où

$u_{D_{P_j,\lambda}}$ ,  $u_{D_{P_j,\Delta\theta}}$ ,  $u_{D_{P_j,\Delta t}}$  et  $u_{D_{P_j,con}}$  sont évalués pour les conditions de fonctionnement;

$u_{D_{P_j,res}}$  est l'incertitude relative de la résolution de la puissance optique définie par  $u_{D_{P_j,res}} = (dP_{\text{TLS},j} / P_{\text{TLS},j}) / 2\sqrt{3}$  ( $dP_{\text{TLS},j}$  est la résolution de la puissance optique du wattmètre optique);

$u_{PM_{P_j}}$  est l'incertitude du wattmètre à la puissance optique  $P_j$  telle qu'elle est décrite dans sa certification;

l'incertitude élargie sur la puissance optique d'étalonnage dans toutes les conditions de fonctionnement  $U_{D_{P_j,op}}$ , avec un facteur d'élargissement  $k$ , est exprimée comme suit:

$$U_{D_{P_j,op}} = k u_{D_{P_j,op}} \quad (27)$$

où

$k$  correspond à un niveau de confiance approprié comme cela est décrit à l'Article A.5.